

UC San Diego

UC San Diego Previously Published Works

Title

Evaluation of Autogenous Engineered Septal Cartilage Grafts in Rabbits: A Minimally Invasive Preclinical Model

Permalink

<https://escholarship.org/uc/item/2wn0183k>

Authors

Kushnaryov, Anton
Yamaguchi, Tomonoro
Briggs, Kristen K
et al.

Publication Date

2014-07-23

DOI

10.1155/2014/415821

Copyright Information

This work is made available under the terms of a Creative Commons Attribution License, available at <https://creativecommons.org/licenses/by/4.0/>

Peer reviewed



Published in final edited form as:

Adv Otolaryngol. ; 2014: 415821-. doi:10.1155/2014/415821.

Evaluation of Autogenous Engineered Septal Cartilage Grafts in Rabbits- A Minimally Invasive Preclinical Model

Anton Kushnaryov, MD^{1,2}, Tomonoro Yamaguchi³, Kristen K. Briggs, PhD⁴, Van W. Wong, BS⁴, Marsha Reuther, MD^{1,2}, Monica Neuman, BS⁵, Victor Lin, BS⁶, Robert L. Sah, MD, ScD⁴, Koichi Masuda, MD³, and Deborah Watson, MD, FACS^{1,2}

¹Division of Otolaryngology-Head and Neck Surgery, University of California, San Diego, La Jolla, California, USA

²Head and Neck Surgery Section, VA San Diego Healthcare System, San Diego, California, USA

³Department of Orthopedic Surgery, University of California, San Diego, La Jolla, California, USA

⁴Department of Bioengineering, University of California, San Diego, La Jolla, California, USA

⁵Creighton University School of Medicine, Omaha, Nebraska, USA

⁶University of North Texas Health Sciences Center, Fort Worth, Texas, USA

Abstract

1. Evaluate safety of autogenous engineered septal neocartilage grafts.
2. Compare properties of implanted grafts versus *in vitro* controls.

Study Design—Prospective, basic science

Setting—Research laboratory

Methods—Constructs were fabricated from septal cartilage and serum harvested from adult rabbits and then cultured *in vitro* or implanted on the nasal dorsum as autogenous grafts for 30 or 60 days. Rabbits were monitored for local and systemic complications. Histological, biochemical and biomechanical properties of implanted and *in vitro* constructs were evaluated and compared.

Results—No systemic or serious local complications were observed. After 30 and 60 days, implanted constructs contained more DNA ($p < 0.01$) and less sGAG per DNA ($p < 0.05$) when compared with *in vitro* controls. Confined compressive aggregate moduli were also higher in implanted constructs when compared with *in vitro* controls ($p < 0.05$) and increased with longer *in vivo* incubation time ($p < 0.01$). Implanted constructs displayed resorption rates of 20–45 percent. Calcium deposition in implanted constructs was observed using alizarin red histochemistry and microtomographic analyses.

Corresponding Author: Anton Kushnaryov University of California, San Diego Division of Otolaryngology-Head and Neck Surgery 3350 La Jolla Village Drive, 112-C San Diego, CA 92161, USA akushnaryov@ucsd.edu Phone: (734)657-5678 Fax: (858) 552-7466.

This project was presented at the annual meeting of the American Academy of Otolaryngology – Head and Neck Surgery, Vancouver, British Columbia, 2013.

Conclusion—Autogenous engineered septal cartilage grafts were well tolerated. As seen in experiments with athymic mice, implanted constructs accumulated more DNA and less sGAG when compared with *in vitro* controls. Confined compressive aggregate moduli were also higher in implanted constructs. Implanted constructs displayed resorption rates similar to previously published studies using autogenous implants of native cartilage. The basis for observed calcification in implanted constructs and its effect on long-term graft efficacy is unknown at this time and will be a focus of future studies.

Keywords

cartilage tissue engineering; human septal cartilage; animal model; New Zealand White rabbit; autologous graft

INTRODUCTION

Craniofacial defects created from tumor resection, traumatic loss, or congenital deformities frequently require complex surgical reconstruction to rebuild missing cartilage and bony support. A variety of autologous, allogeneic and synthetic grafts have traditionally been used to provide structural support in these procedures (1–4). While certainly useful in specific situations, each grafting material has drawbacks. Allogeneic grafts carry the risks of immune rejection and the potential for disease transmission. The use of synthetic materials can be complicated by infection and extrusion. Anecdotally, autologous grafts are favored by many reconstructive surgeons. Cartilaginous autografts are a commonly used structural support medium; various donor sites including rib, auricle and nasal septum are all currently in use (5–7). Nasal septal cartilage offers important advantages over other cartilage types due to its favorable mechanical properties, ease of harvest, and minimal donor site morbidity. However, its use remains limited by several factors. These include the limited amount of tissue available and a predetermined, potentially suboptimal, semi-rigid geometric structure. Tissue engineering of autologous neocartilage offers the potential to generate abundant amounts of cartilage from a small donor specimen, with the ability to create grafts in a variety of customizable shapes and sizes.

Previous studies have demonstrated the ability to successfully create human septal neocartilage constructs from single and pooled donor specimens (8–11). Homicz et al. successfully generated human nasal septal neocartilage constructs from chondrocytes seeded onto a polyglycolic acid scaffold (8). Further studies have refined septal cartilage tissue bioengineering techniques to allow growth of semi rigid three-dimensional constructs from single donor samples using a novel Alginate Recovery Method (ARC) (9–11). Recent research has evaluated the feasibility of implanting these constructs in a murine animal model. Chang et al implanted human nasal septal neocartilage constructs into athymic mice and evaluated biocompatibility and maturation after 30 or 60 days *in vivo*. The grafts demonstrated survival and *in vivo* maturation as evidenced by increased mechanical strength, DNA content and distinct morphological characteristics not seen in nonimplanted controls(12).

At the same time as techniques in the field of tissue engineering, including tissue engineering of nasal septal constructs, were elaborated and refined, a parallel area of research involved animal models of human facial defects developed. The New Zealand White Rabbit has been used as an animal model for decades as a human surrogate to examine a variety of pathologies encountered by the reconstructive surgeon. This animal model has been used to examine facial growth and development (13–16), as well as in evaluating facial implants (17,18). Additionally, de Souza et al used the New Zealand White Rabbit in experiments comparing crushed and uncrushed septal cartilage implants and the effect of crushing on calcification, resorption and viability (19). They found that cartilage, whether autologous or homologous, crushed or uncrushed, demonstrated viability, although fibrous ingrowth was noted when crushed cartilage was implanted. Scierski et al also used this rabbit model to investigate the efficacy of various synthetics used for repair of nasal septal perforations (20). In 2001, Wong et al described an invasive method of rabbit nasal septal cartilage harvest and characterized specific cellular, metabolic and physical properties of the cartilage (21).

Although investigators have used the New Zealand White Rabbit as an animal model and extrapolated these results to humans, no studies to date have used autologous tissue engineered neocartilage constructs in their study design, nor has any study evaluated the feasibility and safety of these constructs. The current study was designed to establish a preclinical animal model for the use of autologous nasal septal neocartilage grafts. Demonstration of safety and efficacy in an animal model is an important prerequisite for undertaking any studies with this technology in humans.

METHODS

Creation of Rabbit Nasal Septal Defect and Harvest of Cartilaginous Septum

A 5×10 mm portion of nasal septum was harvested from sixteen adult female New Zealand White Rabbits near the nasal dorsum according to the following surgical technique: After sedation and intubation the rabbit was placed prone on a heated surgical table. An area of 2×4cm on the midline nasal dorsum was shaved with electric clippers, prepped with povidone iodide solution, and sterilely draped. A 15 mm midline supraperiosteal incision was made over the dorsum. A 20 ×15 mm periosteal flap was raised sharply. An osteotome was used to raise a 10 × 20 mm bone flap which was left anchored rostrally. The upper lateral cartilages were separated from the dorsal nasal septum in continuity with a mucoperichondrial flap. The exposed cartilage was harvested sharply. The upper lateral cartilages were replaced. The bone and periosteal flaps were replaced and the incision closed in layers. During the procedure, each animal's heart rate, respiratory rate, oxygen saturation, reflexes and response to pain was monitored. The length of the procedure was 15–25 minutes per rabbit. All animals were subject to ongoing general health monitoring according to UCSD Institutional Animal Care and Use Committee guidelines.

Creation of cartilage constructs

Each septal specimen was used to fabricate 2–3 autologous neocartilage constructs according to a previously published protocol using the ARC method (10). Although this has

been described briefly, the method is briefly summarized here: The samples we obtain during surgery are cleaned and diced. The chondrocyte fraction is isolated and ultimately plated in a tissue culture flask as a monolayer, using a proprietary culture medium. When the cells are confluent, they are released from the tissue culture flask and suspended in a solution containing low viscosity Alginate. Slowly dripping this solution into a second solution creates 3 dimensional chondrocyte containing Alginate beads. These beads are further cultured and eventually depolymerized. In the final step, free chondrocytes, and the extracellular matrix they have been secreting, are further cultured and matured in tissue wells and become neocartilage constructs. After a culture period of 90 days, the constructs were harvested. Each construct was about 15 mm in diameter by about 2–4 mm thick at the time of harvested. Half of the samples remained in culture as *in vitro* controls. The remaining constructs were implanted as autologous dorsal onlay grafts for a period of 30 or 60 days.

Implantation as autologous nasal dorsal onlay grafts

After confirming adequate sedation, each rabbit was placed prone on a heated surgical table. The nasal dorsum was shaved with electric clippers, prepped with povidone iodide solution and sterilely draped. A 15 mm midline incision over the dorsum was made to a supraperiosteal depth. Blunt dissection generated a precise pocket for implantation. One or two constructs were placed into separate pockets over the rabbit nasal dorsum. The skin and subcutaneous tissue was approximated using resorbable suture. During the procedure, the animal was monitored using the same protocol as the initial surgical procedure. The length of the procedure was 10–15 minutes per animal. On the appropriate experimental day, the animals were sacrificed and each neocartilage construct was recovered for analysis.

Biochemical Evaluation

A small portion of the neocartilage constructs was digested with proteinase K (PK) (Roche Diagnostics, Indianapolis, IN) in phosphate-buffered EDTA for 16 hours. The sGAG content in the PK digests was determined using the dimethyl-methylene blue (DMMB) reaction according to prior published reports (22). GAG content was normalized per gram of wet tissue weight (before digestion) and to DNA content (23). The hydroxyproline assay was used to determine the amount of total collagen in the PK digests according to a previously published protocol (23). Hydroxyproline content was normalized per gram of wet tissue weight (prior to digestion) and to DNA content. The amount of collagen in the sample was estimated using the formula: collagen (g)/(tissue (g) – 7.69 = hydroxyproline (g). The PicoGreen DNA assay was used to determine the amount of DNA in the PK digests according to previously published protocols (24).

Histochemistry

A portion of each construct was placed in OCT compound, frozen by immersion in liquid nitrogen-cooled isopentane and sectioned using a Cryostat (Leica Biosystems, Wetzlar, Germany). The 30–40 micron samples were mounted on poly-L lysine coated slides (Polysciences Inc., Warrington, PA).

Immunohistochemistry was performed with the Vectastain Elite ABC kit (Vector Laboratories, Burlingame, CA), a peroxidase-based detection system, according to the manufacturer's instructions. The samples were probed with one of three antibodies: anti-type I collagen (#ab6308, Abcam, Cambridge, MA) at a concentration of 7 $\mu\text{g}/\text{mL}$, anti-type II collagen (#7005, Chondrex Inc, Redmond, WA) at a concentration of 0.5 $\mu\text{g}/\text{mL}$, or a mouse nonspecific IgG used at 7 $\mu\text{g}/\text{mL}$ as a negative control. Sections were counterstained with methyl green nuclear stain (Vector Laboratories, Burlingame, CA).

To visualize GAG deposition, additional sectioned samples were stained with 0.1% Alcian Blue using standard techniques. Alizarin Red staining was performed to visualize calcium deposition in the sectioned samples according to standard techniques. Samples were documented by photomicroscopy.

Confined Compression Testing

Specimens for mechanical testing were kept hydrated with phosphate buffered saline (PBS) supplemented with calcium, magnesium, and protease inhibitors during testing. The thickness of each construct was measured at 3 points distributed around the circumference and center of each sample, using a non-contact laser displacement sensor ($\pm 0.024\text{mm}$ resolution).

For compression testing, a 4.8 mm diameter disk was isolated from each construct and tested following a previously published protocol (25). The compressive mechanical properties of cartilage samples were calculated from the acquired data assuming tissue homogeneity. The equilibrium-confined compression (aggregate) modulus H_{A0} was estimated by using a least-squares method to fit the equilibrium stress-strain data to a finite deformation constitutive relation, which has been shown previously to provide an excellent fit of compression data (24–27). The permeability k_p at 15% compressive strain was estimated by fitting the measured dynamic stiffness (amplitude and phase) to the theoretical solution using the computed value of H_A at 15% compressive strain.

Statistical Analysis

Statistical analysis was performed using Systat 10.2 (SYSTAT Software Inc., Richmond, CA). Means are presented \pm the standard deviation (SD). Differences in DNA, GAG, collagen and confined compression modulus were assessed using a oneway analysis of variance (ANOVA) to determine the fixed effect of maturation time. If ANOVA identified an overall significant effect, post-hoc Tukey's honestly significant differences (HSD) tests were used to identify significant differences between time points. A $p < 0.05$ was considered significant.

RESULTS

Nasal septal cartilage specimens from sixteen New Zealand White Adult Rabbits were harvested using a minimally invasive surgical technique. The cartilage was used to generate tissue engineered neocartilage constructs which were matured *in vitro* using the ARC method. One half of these constructs were implanted as autologous nasal dorsal onlay grafts and examined after 30 or 60 days, while the other half served as *in vitro* controls.

Histological, biochemical, and biomechanical data were collected for the two onlay graft cohorts and compared with the data collected for the neocartilage constructs which remained as *in vitro* controls.

There was a significant increase in the total DNA content by weight in the *in vivo* neocartilage constructs when compared with the *in vitro* control constructs, at both 30 and 60 days post-implantation. In the 30 day group, the mean DNA content per wet weight was 0.95 ± 0.45 $\mu\text{g}/\text{mg}$ and 0.27 ± 0.10 $\mu\text{g}/\text{mg}$ for the *in vivo* and *in vitro* groups respectively (Figure 1A, $p=0.00$). Similarly, the mean DNA content per wet weight for the *in vivo* and *in vitro* groups at 60 days post-implantation was 0.76 ± 0.33 $\mu\text{g}/\text{mg}$ and 0.23 ± 0.12 $\mu\text{g}/\text{mg}$ respectively (Figure 1A, $p=0.00$).

In contrast, sGAG deposition per DNA decreased in the *in vivo* constructs when compared with *in vitro* control constructs, at both 30 and 60 days. At 30 days post-implantation, the mean sGAG per DNA was 5.70 ± 3.46 $\mu\text{g}/\mu\text{g}$ and 29.5 ± 15.7 $\mu\text{g}/\mu\text{g}$ for the *in vivo* and *in vitro* groups respectively (Figure 1B, $p=0.02$). This compared with 4.27 ± 1.10 $\mu\text{g}/\mu\text{g}$ and 38.8 ± 26.5 $\mu\text{g}/\mu\text{g}$ for the *in vivo* and *in vitro* groups respectively at 60 days post-implantation (Figure 1B, $p=0.00$). In contrast, the total collagen content per DNA remained stable between the *in vivo* and *in vitro* cohorts, at 30 and 60 days post-implantation (data not shown).

Confined compression tests were performed to determine the aggregate modulus (H_{A0}) and the hydraulic permeability (k_0) of each of the neocartilage constructs. H_{A0} is a measure of the tissue stiffness at equilibrium. The higher the H_{A0} , the less the tissue deforms under a given load. H_{A0} values increased in the *in vivo* neocartilage constructs when compared with the *in vitro* control constructs at both 30 and 60 days post-implantation. At 30 days post-implantation, H_{A0} values were 0.263 ± 0.203 MPa and 0.001 ± 0.001 MPa for the *in vivo* and *in vitro* groups respectively (Figure 1C, $p=0.021$). After 60 days post-implantation, H_{A0} values increased to 0.686 ± 0.027 MPa and 0.002 ± 0.001 MPa for the *in vivo* and *in vitro* groups respectively (Figure 1C, $p=0.001$). In addition, there was a significant increase in H_{A0} with increasing *in vivo* incubation time (Figure 1C, $p=0.008$). The transient mechanical behavior of cartilage is related to its interstitial fluid flow which is governed by hydraulic permeability (k_0). In this study, k_0 values at 15, 30 and 45% compression were not significantly different between the neocartilage construct groups (data not shown).

Histologic examination of the neocartilage constructs showed a distribution of chondrocytes in lacunae within an extracellular matrix, typical of native cartilage (30). Histochemical analyses of neocartilage tissue showed deposition of sGAG in both *in vitro* and *in vivo* tissue sections (data not shown). In addition, all constructs accumulated type I and type II collagen (Figure 2). Neocartilage constructs incubated *in vivo* for 30 or 60 days also formed enlarged lacunae containing large numbers of cells (Figures 2 and 3). Furthermore, *in vivo* incubation of the neocartilage constructs resulted in diffuse calcium deposition as visualized by Alizarin Red S staining (Figure 3) and microtomography analyses (data not shown). Light microscopy revealed no evidence of inflammatory infiltrate in the specimens, or gross evidence of a rabbit inflammatory response at any time postoperatively. No ingrowth from

the surrounding tissues was observed. The degree of calcification varied from 20–45%. *In vivo* and *In vitro* specimens at 30 and 60 days are shown in Figure 4.

There were no serious complications in any of the rabbits studied. Out of sixteen rabbits, two had transient, self-limited elevation of the nasal skin flap with expiration after the initial surgical procedure. This resolved after 1–2 days, and produced no long term sequelae. There were no postoperative respiratory problems, no surgical site infections or dehiscence and no other adverse events associated with this experiment.

DISCUSSION

In this study we demonstrated successful *in vivo* implantation and maturation of autologous nasal septal neocartilage constructs. To our knowledge, this is the first reported animal model system for the implantation of wholly autologous tissue engineered cartilage. Previous studies have evaluated autologous native cartilage grafts in animal model systems (19, 29). Bermueller et al recently published an article describing tissue engineered cartilage used in orthotopic rabbit nasal septal defects (33). These constructs used autologous chondrocytes and nonautologous marine collagen scaffolding. Other studies have used implanted human septal chondrocyte-derived constructs in an immune deficient murine model (12). Another recent study by Fulco et al described the implantation of autologous tissue engineered cartilage in the humans, however these constructs were created by embedding chondrocytes in an off-the-shelf, nonautologous collagen matrix (34). By using autologous tissue engineered construct implants, our study serves as a foundation for future studies in animals, leading towards eventual *in vivo* human studies of wholly autologous tissue engineered neocartilage grafts.

To date, the literature also does not report any detailed, reproducible, minimally-invasive surgical approach through the nasal vault for harvesting septal cartilage. Gubisch et al have described a more invasive technique involving multiple incisions including hemitransfixion incisions (30). Wong et al described an approach which involved a larger skin incision, more extensive dissection, and the use of power instrumentation to create a larger bone flap (21). Using the minimally invasive technique described in the current study, the rabbits displayed no significant respiratory issues or long term post-operative deficits. In addition, no surgical site infections or wound dehiscence occurred. This study serves to establish the feasibility of a minimally invasive surgical procedure, using the New Zealand White rabbit as an animal model, for autologous tissue engineered nasal septal neocartilage grafts. It also demonstrates the safety of the reimplanted neocartilage constructs. No adverse events were observed in either experimental group. The post-surgical implant sites did not show evidence of graft rejection, infection, capsule formation, or other undesired features.

DNA content, a surrogate measure of cell number, was higher in the *in vivo* than in the *in vitro* neocartilage constructs at both 30 and 60 days post-implantation. We postulate that the increase in DNA in the *in vivo* group reflects a change in the constructs reflecting increased cellularity associated with maturation in the complex environment within the rabbit. In contrast sGAG accumulation per DNA, a proxy for the amount of proteoglycan contained in cartilage tissue, decreased significantly after *in vivo* implantation. This correlates with the

increased DNA content seen in the *in vivo* constructs. An increase in DNA and decrease in sGAG content were also observed when tissue engineered human nasal septal neocartilage constructs were subjected to a period of maturation *in vivo* after implantation in nude mice (12). In contrast to the nude mouse implantation study, *in vivo* maturation did not enhance collagen levels in the current work. Differences in collagen levels between these two studies may be due to the methods used to measure collagen levels. In the current study, the hydroxyproline assay was used to measure total collagen, while ELISA was used to determine solubilized type II collagen in the nude mouse study. Another explanation for the differences in collagen level between the two studies may be the presence of calcium deposition and chondrocyte hypertrophy observed in the implanted rabbit neocartilage tissue.

Implantation of autologous neocartilage constructs resulted in significant gains in mechanical stiffness. The aggregate moduli (H_{A0}) increased in the *in vivo* neocartilage constructs when compared with the *in vitro* control constructs at both 30 and 60 days post-implantation. Additional gains in stiffness were observed with increasing time of *in vivo* incubation.

Histological examination of the autologous tissue engineered neocartilage constructs revealed chondrocytes nestled in lacunae and distributed within an extracellular matrix as seen in native nasal septal cartilage (32). Alcian Blue staining of *in vitro* and *in vivo* incubated neocartilage constructs showed accumulation of GAG at 30 and 60 days post-implantation and all neocartilage constructs expressed both type I and type II collagen. It was noted, however, that diffuse calcium deposition and minor resorption based on construct diameter in the *in vivo* implants was present. Previously published research by Lattyak et al demonstrated resorption rates of up to 30% in rabbits implanted with autologous septal cartilage (29). They implanted autologous septal, auricular and costal cartilage as dorsal onlay grafts and observed resorption rates of 30.8% in septal cartilage, 21.3% in auricular cartilage and 7.6% in costal cartilage. Another study by de Souza et al evaluating rabbit autologous septal grafts demonstrated no calcification of the graft, but did report resorption rates of 15–50% (19). Since this study is the first report demonstrating implantation of autologous rabbit septal cartilage constructs, it is difficult to compare rates of calcification and resorption to experiments using crushed or uncrushed native rabbit septal cartilage. Furthermore, it is unknown whether this resorption would be balanced by the formation of a fibrous capsule, as has been suggested by some authors (19, 31).

This study has demonstrated a reliable non-invasive surgical approach to the rabbit septum, and the utility of the rabbit model. This can be very useful in future investigations to evaluate the longevity of tissue engineered constructs in the *in vivo* setting.

Acknowledgments

This material is based upon work supported in part by the Department of Veterans Affairs, Veterans Health Administration, Office of Research and Development (BL R&D Merit Award (D.W.), NIH R01 AR044058 (R.L.S.) and the American Academy of Otolaryngology – Head and Neck Surgery Foundation Resident Research Award (A.K)

References

1. Berlang T, Runeson P. Efficient evaluation of multifactor dependent system performance using fractional factorial design. *IEEE Trans Software Eng.* 2003; 29:769–781.
2. Tardy ME Jr, Denny J III, Fritsch MH. The versatile cartilage autograft in reconstruction of the nose and face. *Laryngoscope.* 1985; 95:523–33. [PubMed: 3990484]
3. Komender J, Marczynski W, Tylman D. Preserved tissue allografts in reconstructive surgery. *Cell Tissue Bank.* 2001; 2:103–12. [PubMed: 15256921]
4. Lovice DB, Mingrone MD, Toriumi DM. Grafts and implants in rhinoplasty and nasal reconstruction. *Otolaryngol Clin North Am.* 1999; 32:113–41. [PubMed: 10196441]
5. Moretti A, Sciuto S. Rib grafts in septorhinoplasty *Acta Otorhinolaryngol Ital.* Jun; 2013 33(3):190–5. PMID: 23853415.
6. Son D, Kwak M, Yun S, Yeo H, Kim J, Han K. Large auricular chondrocutaneous composite graft for nasal alar and columellar reconstruction. *Arch Plast Surg.* Jul; 2012 39(4):323–8. doi: 10.5999/aps.2012.39.4.323. [PubMed: 22872834]
7. Lin J, Chen X, Wang X, Gao X, Zheng X, Chen X, Yuan Y. *JAMA Facial Plast Surg.* Jul 25, 2013 A Modified Septal Extension Graft for the Asian Nasal Tip. doi: 10.1001/jamafacial.2013.1285.
8. Homicz MR, Schumacher BL, Sah RL, Watson D. Effects of serial expansion of septal chondrocytes on tissue-engineered neocartilage composition. *Otolaryngol Head Neck Surg.* Nov; 2002 127(5):398–408. [PubMed: 12447233]
9. Masuda K, Miyazaki T, Pfister B, Horvath E, Thonar EJ-M. Human tissue engineered cartilage by the alginate-recovered-chondrocyte method after an expansion in monolayer. *Trans Orthop Res Soc.* 2002; 27:467.
10. Masuda K, Sah RL, Hejna MJ, Thonar EJ-M. A novel two-step method for the formation of tissue engineered cartilage: The alginate-recovered-chondrocyte (ARC) method. *J Orthop Res.* 2003; 21(1):139–48. [PubMed: 12507591]
11. Chia SH, Schumacher BL, Klein TJ, Thonar EJ, Masuda K, Sah RL, Watson D. Tissue-engineered human nasal septal cartilage using the alginate-recovered-chondrocyte method. *Laryngoscope.* Jan; 2004 114(1):38–45. [PubMed: 14709992]
12. Chang AA, Reuther MS, Briggs KK, Schumacher BL, Williams GM, Corr M, Sah RL, Watson D. In vivo implantation of tissue-engineered human nasal septal neocartilage constructs: a pilot study. *Otolaryngol Head Neck Surg.* Jan; 2012 146(1):46–52. [PubMed: 22031592]
13. Nolst Trenite GJ, Verwoerd Verwoerd-Verhoef. Reimplantation of autologous septal cartilage in the growing nasal septum I. The influence of resection and reimplantation of septal cartilage upon nasal growth: An experimental study in rabbits. *Rhinology.* 1987; 25:225–36. [PubMed: 3432924]
14. Nolst Trenite GJ, Verwoerd Verwoerd-Verhoef. Reimplantation of autologous septal cartilage in the growing nasal septum II. The influence of reimplantation of rotated or crushed autologous septal cartilage on nasal growth: An experimental study in rabbits. *Rhinology.* 1987; 25:225–36. [PubMed: 3432924]
15. Verwoerd CD, Urbanus NA, Nijdam DC. The effects of septal surgery on the growth of nose and maxilla. *Rhinology.* 1979; 17:53–63. [PubMed: 493820]
16. Verwoerd CD, Urbanus NA, Mastenbroek GJ. The influence of partial resections of the nasal septal cartilage on the growth of the upper jaw and the nose: An experimental study in rabbits. *Clin. Otolaryngol.* 1980; 5:290–30.
17. Kramp B, Bernd HE, Schumacher WA, Blynow M, Schmidt W, Kunze C, Behrend D, Schmitz KP. [Poly-beta-hydroxybutyric acid (PHB) films and plates in defect covering of the osseous skull in a rabbit model]. *Laryngorhinootologie.* May; 2002 81(5):351–6. [PubMed: 12001025]
18. Oliveira RV, de Souza Nunes LS, Filho HN, de Andrade Holgado L, Ribeiro DA, Matsumoto MA. Fibrovascularization and osteogenesis in high-density porous polyethylene implants. *J Craniofac Surg.* Jul; 2009 20(4):1120–4. [PubMed: 19553849]
19. de Souza MMA, Gregório LC, Sesso R, Souza SA, Settanni F. Study of rabbit septal cartilage grafts placed on the nasal dorsum. *Archives of Facial Plastic Surgery.* 2008; 10(4):250–254. [PubMed: 18645093]

20. cierski W, Polok A, Namysłowski G, Bła ewicz M, Pamuła E, Stodolak E, No y ski J, wirska-Korczała K, Szwarz K, Misiółek M, Czecior E, Turecka L, Lisowska G, Orecka B. Ocena wybranych biomateriałów do rekonstrukcji perforacji przegrody nosa. *Otolaryngologia Polska*. 2007; 61(5):842–846. ISSN 0030-6657.
21. Wong BJ, Chao KK, Kim HK, Chu EA, Dao X, Gaon M, Nelson JS. The porcine and lagomorph septal cartilages: models for tissue engineering and morphologic cartilage research. *American journal of rhinology*. 2001; 15(2):109–116. [PubMed: 11345149]
22. Farndale RW, Buttle DJ, Barrett AJ. Improved quantitation and discrimination of sulphated glycosaminoglycans by use of dimethylmethylene blue. *Biochim Biophys Acta*. 1986; 883:173–177. Medline. [PubMed: 3091074]
23. Jackson DS, Cleary EG. The determination of collagen and elastin. *Methods Biochem Anal*. 1967; 15:25–76. Medline. [PubMed: 4899619]
24. McGowan KB, Kurtis MS, Lottman LM, Watson D, Sah RL. Biochemical quantification of DNA in human articular and septal cartilage using PicoGreen and Hoechst 33258. *Osteoarthritis Cartilage*. Jul; 2002 10(7):580–587. [PubMed: 12127839]
25. Richmon JD, Sage A, Wong VW, Chen AC, Sah RL, Watson D. Compressive biomechanical properties of human nasal septal cartilage. *American Journal of Rhinology*. 2006; 20:1–20. [PubMed: 16539286]
26. Chen AC, Bae WC, Schinagl RM, Sah RL. Depth- and strain-dependent mechanical and electromechanical properties of full-thickness bovine articular cartilage in confined compression. *J Biomech*. Jan; 2001 34(1):1–12. [PubMed: 11425068]
27. Williamson AK, Chen AC, Sah RL. Compressive properties and function-composition relationships of developing bovine articular cartilage. *J Orthop Res*. Nov; 2001 19(6):1113–1121. [PubMed: 11781013]
28. Schinagl RM, Gurskis D, Chen AC, Sah RL. Depth-dependent confined compression modulus of full-thickness bovine articular cartilage. *J Orthop Res*. Jul; 1997 15(4):499–506. [PubMed: 9379258]
29. Lattyak BV, Maas CS, Sykes JM. Dorsal Onlay Cartilage Autografts. Comparing Resorption in an Animal Model. *Arch Facial Plast Surg*. May-Jun;2003 5(3):240–3. [PubMed: 12756118]
30. Gubisch W, Greulich M, Donath K. Experimental and Clinical Study on the Vitality of Orthotopic Cartilage Implants. *Plast Reconstr Surg*. 1995; 95:663–671. [PubMed: 7892310]
31. Adlington P, Anscombe AJ, Phillips JJ. Influence of the mode of preparation on the long-term efficacy of homologous costal cartilage implants. *J Laryngol Otol*. 1992; 106(6):511–517. [PubMed: 1624886]
32. Vetter U, Pirsig W, Helbing D, Heit W, Heinze E. Patterns of growth in human septal cartilage: a review of new approaches. *International Journal of Pediatric Otorhinolaryngology*. 1984; 7:63–74. [PubMed: 6724811]
33. Bermueller C, Schwarz S, Elsaesser AF, Sewing J, Baur N, von Bomhard A, Scheithauer M, Notbohm H, Rotter N. Marine collagen scaffolds for nasal cartilage repair: prevention of nasal septal perforations in a new orthotopic rat model using tissue engineering techniques. *Tissue Eng Part A*. Oct; 2013 19(19–20):2201–14. [PubMed: 23621795]
34. Fulco I, Miot S, Haug MD, Barbero A, Wixmerten A, Feliciano S, Wolf F, Jundt G, Marsano A, Farhadi J, Heberer M, Jakob M, Schaefer DJ, Martin I. Engineered autologous cartilage tissue for nasal reconstruction after tumour resection: an observational first-in-human trial. *Lancet*. Apr 9.2014 pii: S0140-6736(14)60544-4.

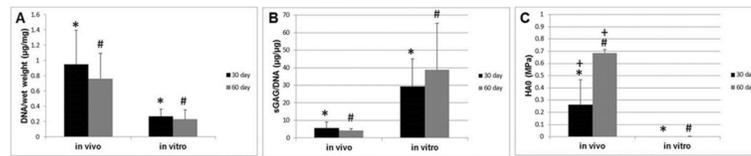


Figure 1.

Biochemical and biomechanical characterization of implanted and control constructs after 30 or 60 days. Implanted *in vivo* constructs accumulated more DNA per wet weight (A) and less sGAG per DNA (B) than the *in vitro* control constructs. The aggregate modulus (H_{A0}) was also greater for implanted constructs when compared with the *in vitro* control constructs (C). In addition, H_{A0} increased upon increasing time of *in vivo* incubation (D). * $p < 0.05$, # $p < 0.01$, + $p = 0.008$

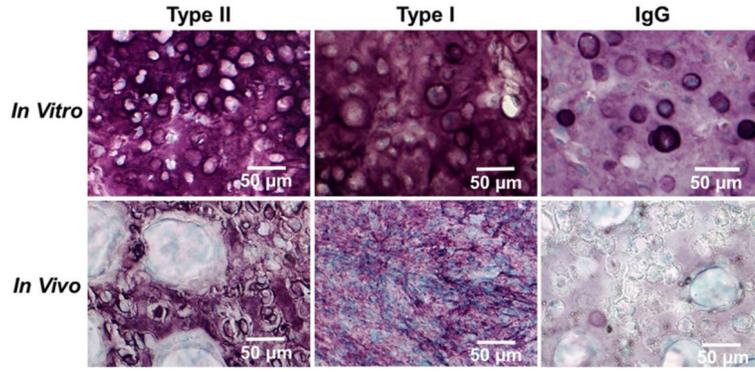


Figure 2. Immunohistochemical staining for type I and type II collagen in *in vitro* control neocartilage constructs (top) or after 30 days *in vivo* (below). Sections were counterstained with the nuclear stain methyl green. Neocartilage constructs had robust staining for both collagen types II and I (left and middle) compared with the non-specific control IgG (right). In addition, *in vivo* tissue had enlarged lacunae containing large clusters of cells.

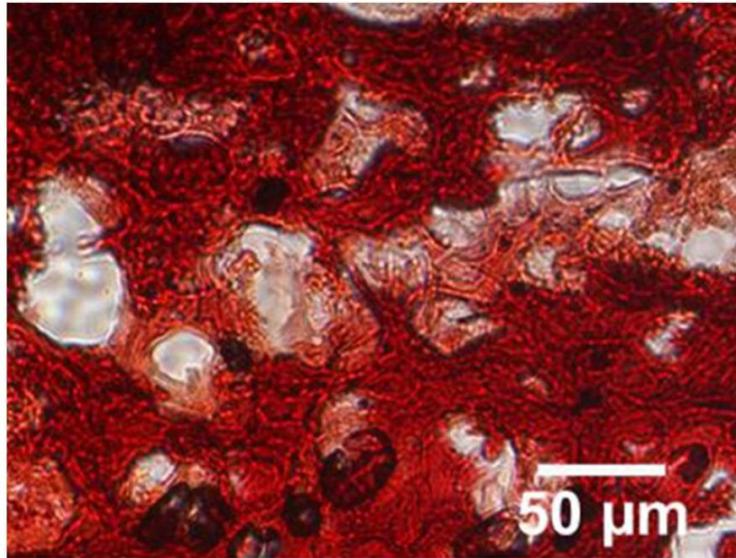


Figure 3. Alizarin Red S staining confirmed deposition of calcium in neocartilage constructs after 30 days implantation.

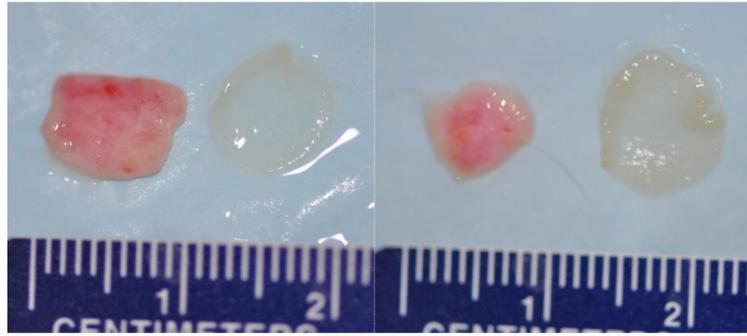


Figure 4. Representative photographs of *in vivo* and *in vitro* constructs at 30 and 60 days are shown. Measurements are in centimeters.