

# Lawrence Berkeley National Laboratory

## Recent Work

### Title

A METHOD FOR MAPPING THE SPATIAL DISTRIBUTION OF STOPPING  $n$  MESONS IN TISSUE

### Permalink

<https://escholarship.org/uc/item/360526j5>

### Authors

Miller, A.J.  
Raju, M.R.  
Rindi, A.  
et al.

### Publication Date

1969-10-30

Presented at the Boulder Meeting  
of the Los Alamos Users Group  
Boulder, Colorado  
October 30-November 1, 1969.


UCRL-19376  
Preprint c.2 repl.

A METHOD FOR MAPPING THE SPATIAL DISTRIBUTION  
OF STOPPING  $\pi^-$  MESONS IN TISSUE

A. J. Miller, M. R. Raju, A. Rindi, V. Perez-Mendez, and  
J. Sperinde

October 30, 1969

AEC Contract No. W-7405-eng-48

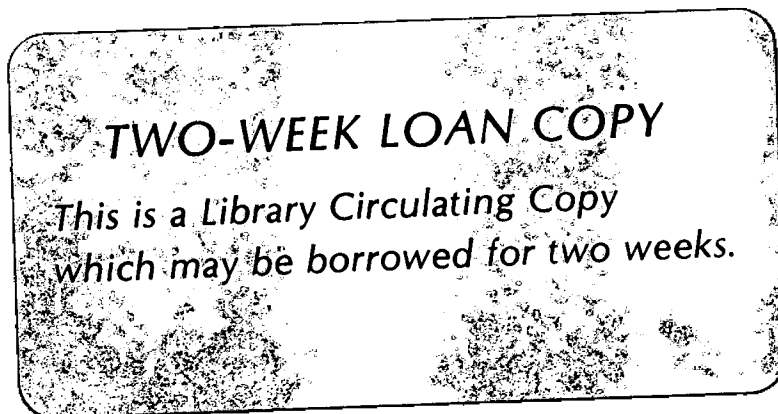

LAWRENCE RADIATION LABORATORY  
UNIVERSITY of CALIFORNIA BERKELEY

UCRL-19376  
c.2 repl.

## **DISCLAIMER**

This document was prepared as an account of work sponsored by the United States Government. While this document is believed to contain correct information, neither the United States Government nor any agency thereof, nor the Regents of the University of California, nor any of their employees, makes any warranty, express or implied, or assumes any legal responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by its trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof, or the Regents of the University of California. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof or the Regents of the University of California.

Presented at the Boulder Meeting  
of the Los Alamos Users Group,  
October 30-November 1, 1969.

UCRL-19376  
Preprint

A METHOD FOR MAPPING THE SPATIAL DISTRIBUTION  
OF STOPPING  $\pi^-$  MESONS IN TISSUE

A. J. Miller, M. R. Raju, A. Rindi, V. Perez-Mendez, and J. Sperinde

October 30, 1969

AEC Contract No. W-7405-eng-48

A METHOD FOR MAPPING THE SPATIAL DISTRIBUTION  
OF STOPPING  $\pi^-$  MESONS IN TISSUE \*

A. J. Miller, M. R. Raju, A. Rindi, V. Perez-Mendez, and J. Sperinde

Stopping  $\pi^-$  beams have been proposed<sup>1,2,3</sup> for radiotherapeutic applications in view of the fact that the 'star' formation in the capture reaction produces a highly localized dense ionization region. This is of interest as a possible method for the treatment of deep-seated tumors containing anoxic cells.

Due to inhomogeneities in the average density of bone and tissue layers in each patient, it may be difficult to locate the exact position of the capture star formation region in the patient's tumor. This difficulty also exists in other methods of radiation treatment using Bragg peak ionization effects. Pi minus mesons have an advantage in this respect in view of the fact that  $\gamma$ -rays are emitted in the capture process. In this paper we describe the use of the capture  $\gamma$ -rays for the purpose of mapping the stopping region.

In addition to the emission of charged particles from star events, about 2% of stopping pions produce high energy  $\gamma$ 's, peaking in the energy region of 100 MeV.<sup>4</sup> Calculations of the capture of negative pions by Guthrie et al.,<sup>5</sup> indicate an average excitation energy of about 5 MeV, that will be emitted as  $\gamma$ -rays. In addition to these pi-mesic X-rays will also be emitted.

In the present investigation  $\gamma$ -rays of energy greater than  $\sim 15$  MeV were detected using the apparatus shown in Figure 1. A Pb collimator is used in order to specify the direction from which the  $\gamma$ 's are coming. The collimator consists of 3 mm sheets of Pb separated by 3 mm gaps, and has a

thickness of 25 cm. After passing through the collimator the  $\gamma$ -rays are converted into electrons by a 3 mm thick lead converter. These electrons traverse the chamber and are detected by a pair of scintillators separated by a 2.5 cm aluminum absorber which requires that the electrons have an energy of at least 15 MeV to traverse the full distance. The coincidence signal from these two scintillators and from a beam monitor scintillator triggers the wire spark chamber. The position of the spark is determined by the magnetostrictive readout technique. The chamber consists of two grids of wires with a wire separation 1 mm and a grid separation of 1 cm which gives a spatial resolution for particles normal to the chamber of about .25 mm. In the present application, the spatial resolution of the system is  $\approx 6$  mm and is determined by the spacing of the lead plates in the collimator.

The measured distributions are shown below in Figure 2. The three peaks are those produced by the successive addition of 6 mm slabs of lucite absorber which displace the stopping region by the same amount. The  $\gamma$ -ray distributions shown on the upstream side of the stopped meson peaks are presumably due to captures in flight.

The overall sensitivity of the system can be gauged from the measured ratio  $S$  of detected  $\gamma$ -rays to stopping pions. In our experimental arrangement  $S = 5 \times 10^{-6}$ . Hence, it would be possible to locate the stopping pion region in a patient with a dose much smaller than the treatment dose.

In addition to the capture  $\gamma$ -rays that we have used in this measurement, it is also possible to use the pi-mesic X-rays emitted in the cascade process prior to nuclear capture. For this purpose we propose to use Silicon detectors. A further intriguing possibility is also available; a small fraction of the  $\pi^-$  ( $\sim 1\%$ ) will produce  $\pi^0$  mesons by charge exchange

on protons. The two 65 MeV  $\gamma$ -rays emitted at  $180^\circ$  to each other can be used--without collimators--to locate the stopping region by using two spark chambers in a similar fashion to that used for positron annihilation  $\gamma$ -rays.

Footnote and References

- \* This work was done under the auspices of the U. S. Atomic Energy Commission.
1. P. H. Fowler, D. H. Perkins, The Possibility of Therapeutic Applications of Beams of Negative  $\pi^-$  Mesons, Nature 189, 524-528 (1961).
  2. C. Richman, H. Aceto Jr., M. R. Raju, B. Schwartz, The Radiotherapeutic Possibilities of Negative Pions. Preliminary Physical Measurements. Am. J. Roentgenol. 96, 777-790 (1966).
  3. M. R. Raju, C. Richman, Physical and Radiobiological Aspects of Negative Pions with Reference to Radiotherapy. Presented at the XII International Congress of Radiology October 6-11, 1969, Tokyo, Japan. To be published in GANN Monograph on Radiology of Cancer; UCRL-18806.
  4. H. Davies, U. Muirhead, J. N. Woulds, High Energy Gamma Rays from Pion Capture. Nucl. Phy. 78, 673-680 (1966).
  5. M. P. Guthrie, R. G. Alsmiller Jr., H. W. Bertini, Calculation of the Capture of Negative Pions in Light Elements and Comparison with Experiments Pertaining to Cancer Radiotherapy. Nucl. Instr. Methods 66, 29-36 (1968).



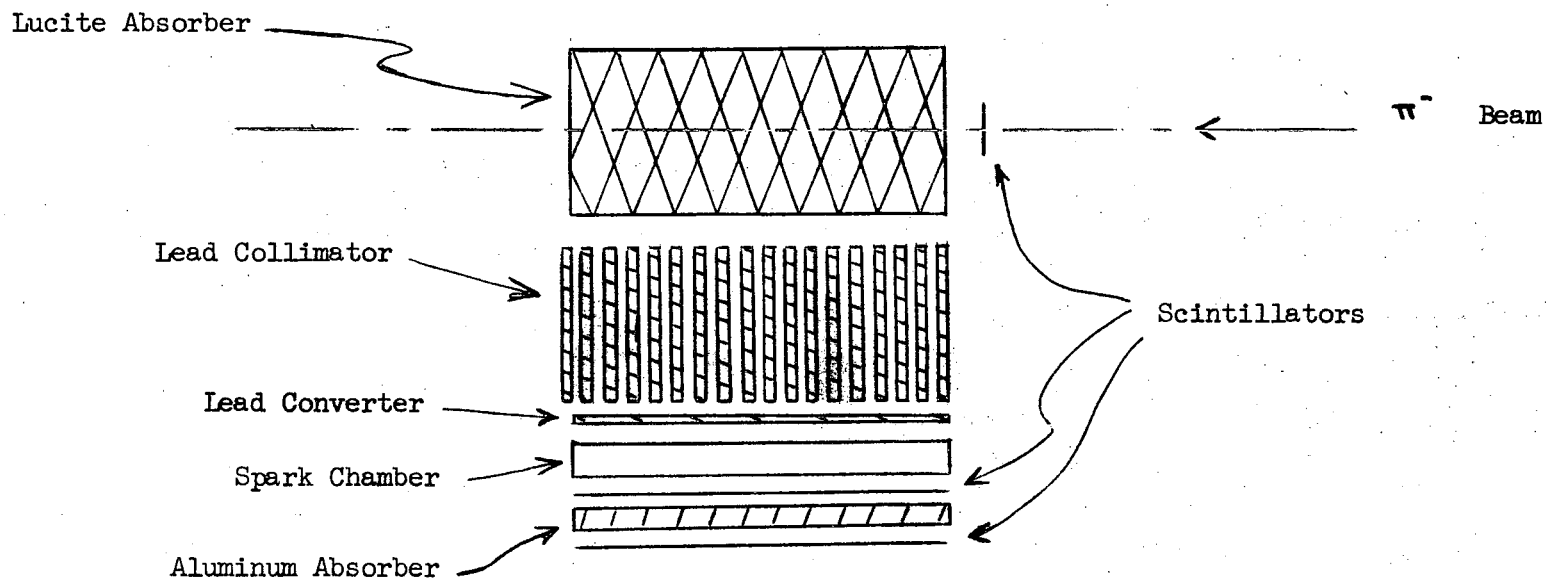


Figure 1. Experimental Set-up.

Number of Gammas (arbitrary units)

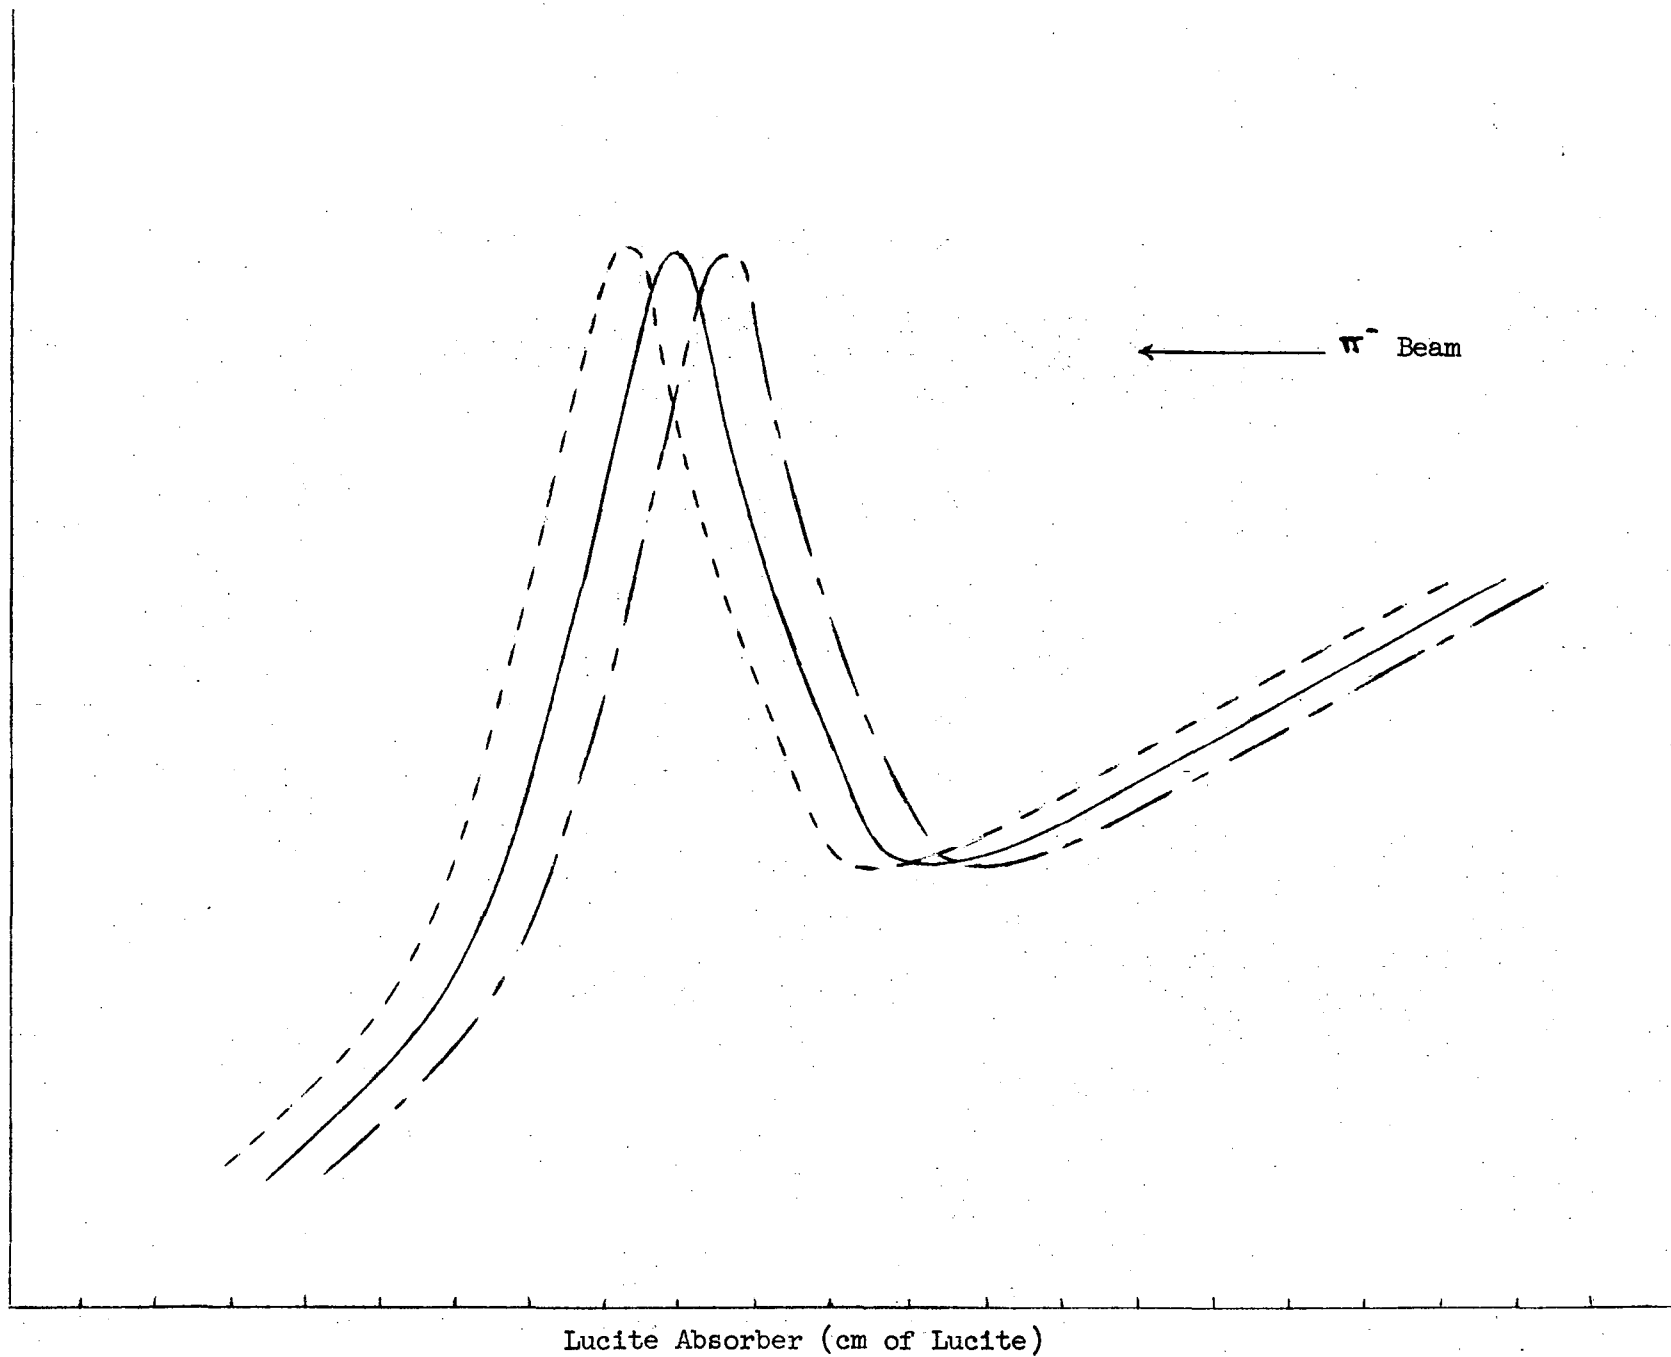


Figure 2. Number of gammas detected as a function of lucite absorber. The dashed curves are obtained by alternately adding or removing 6 mm of lucite.

LEGAL NOTICE

*This report was prepared as an account of Government sponsored work. Neither the United States, nor the Commission, nor any person acting on behalf of the Commission:*

- A. Makes any warranty or representation, expressed or implied, with respect to the accuracy, completeness, or usefulness of the information contained in this report, or that the use of any information, apparatus, method, or process disclosed in this report may not infringe privately owned rights; or*
- B. Assumes any liabilities with respect to the use of, or for damages resulting from the use of any information, apparatus, method, or process disclosed in this report.*

*As used in the above, "person acting on behalf of the Commission" includes any employee or contractor of the Commission, or employee of such contractor, to the extent that such employee or contractor of the Commission, or employee of such contractor prepares, disseminates, or provides access to, any information pursuant to his employment or contract with the Commission, or his employment with such contractor.*

TECHNICAL INFORMATION DIVISION  
LAWRENCE RADIATION LABORATORY  
UNIVERSITY OF CALIFORNIA  
BERKELEY, CALIFORNIA 94720