

Lawrence Berkeley National Laboratory

Recent Work

Title

THE DETECTION OF ARTIFICIALLY PRODUCED PHOTOMESONS WITH COUNTERS

Permalink

<https://escholarship.org/uc/item/7gs144rc>

Authors

Steinberger, J.
Bishop, A.S.

Publication Date

1950-03-08

UCRL 631
4.2

UNCLASSIFIED

UNIVERSITY OF
CALIFORNIA

Radiation Laboratory

TWO-WEEK LOAN COPY

*This is a Library Circulating Copy
which may be borrowed for two weeks.
For a personal retention copy, call
Tech. Info. Division, Ext. 5545*

BERKELEY, CALIFORNIA

DISCLAIMER

This document was prepared as an account of work sponsored by the United States Government. While this document is believed to contain correct information, neither the United States Government nor any agency thereof, nor the Regents of the University of California, nor any of their employees, makes any warranty, express or implied, or assumes any legal responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by its trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof, or the Regents of the University of California. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof or the Regents of the University of California.

UNCLASSIFIED

UNIVERSITY OF CALIFORNIA

Radiation Laboratory

Contract No. W-7405-eng-48

THE DETECTION OF ARTIFICIALLY PRODUCED PHOTOMESONS WITH COUNTERS

J. Steinberger and A. S. Bishop

March 8, 1950

Berkeley, California

-2-

<u>INSTALLATION</u>	<u>No. of Copies</u>
Argonne National Laboratory	8
Armed Forces Special Weapons Project	1
Atomic Energy Commission, Washington	2
Battelle Memorial Institute	1
Brookhaven National Laboratory	8
Bureau of Medicine and Surgery	1
Bureau of Ships	1
Carbide & Carbon Chemicals Corp. (K-25)	4
Carbide & Carbon Chemicals Corp. (Y-12)	4
Chicago Operations Office	1
Cleveland Area Office	1
Columbia University (Dunning)	2
Columbia University (Failla)	1
Dow Chemical Company	1
General Electric Company, Richland	6
Idaho Operations Office	1
Iowa State College	2
Kansas City	1
Kellex Corporation	2
Knolls Atomic Power Laboratory	4
Los Alamos	3
Mallinckrodt Chemical Works	1
Massachusetts Institute of Technology (Gaudin)	1
Massachusetts Institute of Technology (Kaufmann)	1
Mound Laboratory	3
National Advisory Committee for Aeronautics	2
National Bureau of Standards	2
Naval Radiological Defense Laboratory	2
NEPA Project	2
New Brunswick Laboratory	1
New York Operations Office	3
North American Aviation, Inc.	1
Oak Ridge National Laboratory	8
Patent Advisor, Washington	1
Rand Corporation	1
Sandia Base	1
Sylvania Electric Products, Inc.	1
Technical Information Branch, ORE	15
U. S. Public Health Service	1
UCLA Medical Research Laboratory (Warren)	1
University of California Radiation Laboratory	5
University of Rochester	2
University of Washington	1
Western Reserve University (Friedell)	2
Westinghouse	4
Total	117
Information Division	
Radiation Laboratory	
Univ. of California	

-3-

THE DETECTION OF ARTIFICIALLY PRODUCED PHOTOMESONS WITH COUNTERS

J. Steinberger and A. S. Bishop
Radiation Laboratory, Department of Physics
University of California, Berkeley, California

March 8, 1950

Until recently, artificially produced mesons were detected only in photographic plates. Alvarez was the first to detect at least the positive mesons with counters.¹ This technique, which depends on the decay electron for the identification of the meson, was first introduced by Rasetti² in the study of cosmic ray mesons. It has been extensively used in cosmic ray research, and has now, with some modifications, been applied to the photomesons produced by the synchrotron.

When a positive π -meson comes to rest, it disintegrates very quickly into a μ -meson, and this in turn into an electron with the well-known 2.1×10^{-6} sec. mean life. The range of the μ -meson is only $\sim .2g$, so that when this process takes place in a scintillation crystal with linear dimensions of the order of several centimeters, a large fraction of the decay electrons will also appear in the crystal. The $\pi \rightarrow \mu$ decay is too rapid to be resolved in the electronics of the experiment; instead, the characteristic half life of the $\mu \rightarrow e$ decay is used to identify the meson.

The apparatus is sketched in Fig. 1. A meson is counted if it produces pulses simultaneously in crystals I and II, but not in crystal III, and if its decay electron falls into one of several successive

¹ L. W. Alvarez, A. Longacre, V. G. Ogren, R. E. Thomas, Bull. Am. Phys. Soc., Vol. 24, No. 7.

² F. Rasetti, Phys. Rev. 60, 198 (1941).

-4-

delay channels of about 2×10^{-6} sec. time width. There will, of course, be accidental delayed coincidences, but these can be calculated from the known single counting rates, gate width, and duty cycle, and can therefore be subtracted. Usually this background is approximately 10 - 20 percent of the counting rate in the first channel.

After the background subtraction, the counting rates in the several delay channels should reproduce the exponential $\mu - e$ decay. The lifetime data so far obtained are plotted in Fig. 2.

The stability of the detecting system depends on the sensitivity of the meson counting rate to the pulse height of the three scintillation pulses. One of these plateau curves is shown in Fig. 3.

With the usual synchrotron beam intensity of about 10^4 ergs/sec. and the geometry of Fig. 1, the meson counting rate is about 15 counts/min. This makes it possible to do experiments more quickly than with photographic emulsions. On the other hand, so far only positive mesons can be counted in this manner, and absolute cross sections measurements have a large error, since the detection efficiency is not known with precision.

We should like to express our thanks to Professor E. McMillan for his support of this research, and to the operating crew of the synchrotron, especially to Mr. W. Gibbins, for its expert help.

This work was sponsored under the auspices of the Atomic Energy Commission.

Information Division
ead/3-9-50

Figure Captions

- Fig. 1 Arrangement of target, absorbers, and meson detection scintillation counter telescope.
- Fig. 2 Relative counting rates in the delayed channels. Two sets of data are shown because three channels were used at first, later four.
- Fig. 3 Counting rate in crystal II (points without statistical error) and meson counting rate (with mean statistical error indicated) as a function of the minimum voltage required of the first pulse in crystal II.

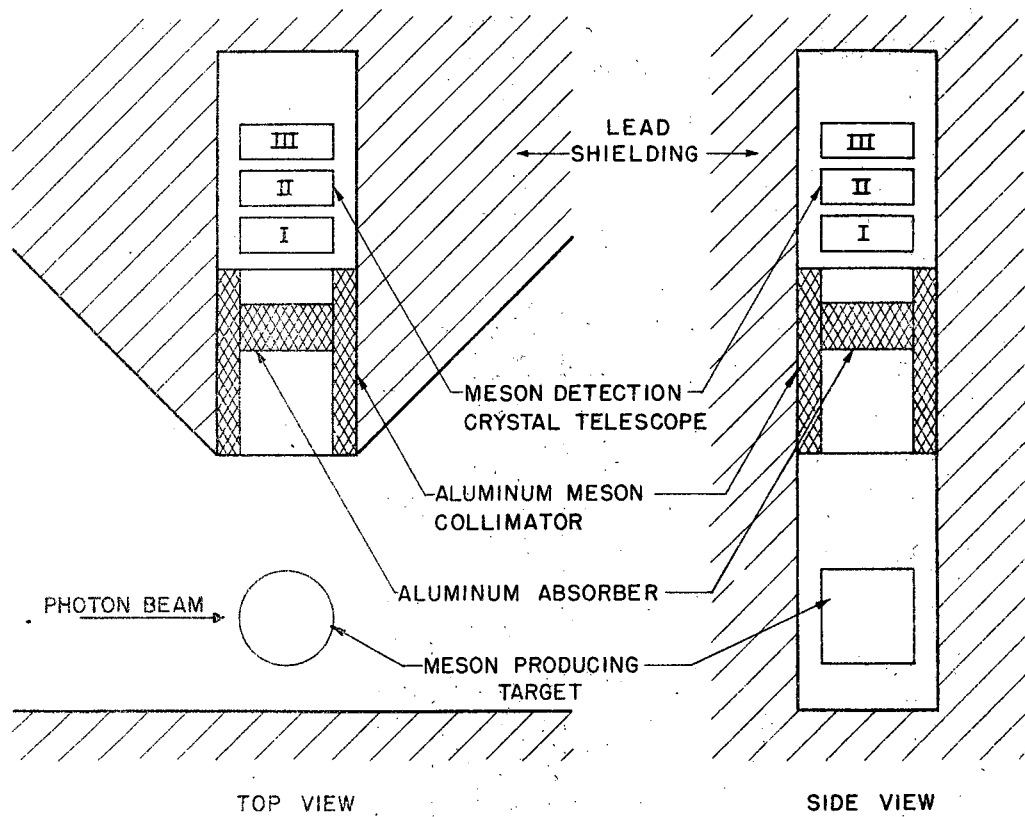


FIG. 1

Mu 67

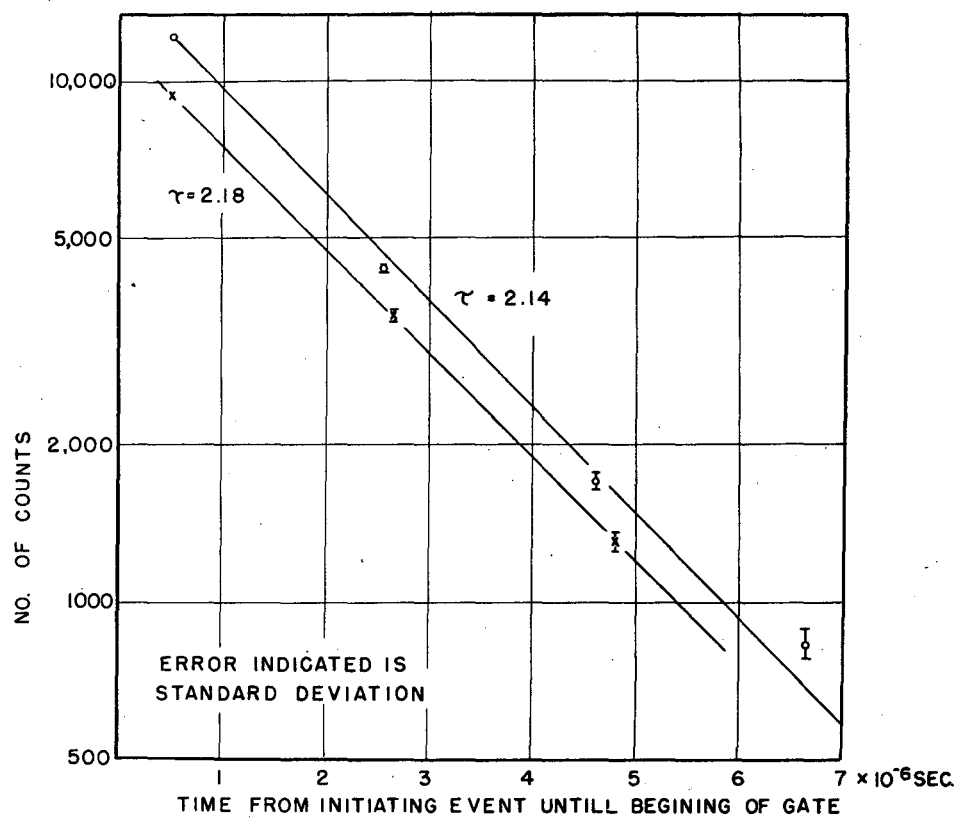


FIG. 2

