

Lawrence Berkeley National Laboratory

Recent Work

Title

NEUTRON RADIOGRAPHY WITH A MULTIWIRE PROPORTIONAL CHAMBERuA STATUS REPORT

Permalink

<https://escholarship.org/uc/item/0538088c>

Authors

Valentine, Kenneth
Perez-Mendez, Victor
Kaufman, Leon
et al.

Publication Date

1973-02-01

Submitted to American Nuclear
Society Meeting, Chicago, IL.,
June 10-15, 1973

LBL-1582
Summary

c.1

NEUTRON RADIOGRAPHY WITH A MULTIWIRE
PROPORTIONAL CHAMBER--A STATUS REPORT

RECEIVED

JAN 25 1973
RADIATION PHYSICS

Kenneth Valentine, Victor Perez-Mendez,
Leon Kaufman, and Selig Kaplan

MAY 11 1973


LIBRARY AND
DOCUMENTS SECTION

February 1973

Prepared for the U.S. Atomic Energy Commission
under Contract W-7405-ENG-48

For Reference

Not to be taken from this room

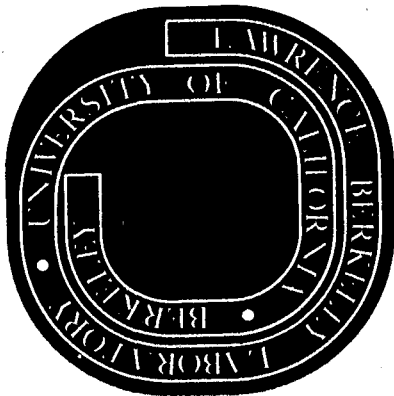

LBL-1582 Summary

DISCLAIMER

This document was prepared as an account of work sponsored by the United States Government. While this document is believed to contain correct information, neither the United States Government nor any agency thereof, nor the Regents of the University of California, nor any of their employees, makes any warranty, express or implied, or assumes any legal responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by its trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof, or the Regents of the University of California. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof or the Regents of the University of California.

LBL-1582
Summary

NEUTRON RADIOGRAPHY WITH A MULTIWIRE PROPORTIONAL
CHAMBER--A STATUS REPORT

Kenneth Valentine, ^{*†} Victor Perez-Mendez ^{*‡}
Leon Kaufman, [‡] and Selig Kaplan ^{*†}

February 1973

* Lawrence Berkeley Laboratory, Berkeley.

† Department of Nuclear Engineering, University of California, Berkeley.

‡ Department of Radiology, University of California, San Francisco.

NEUTRON RADIOGRAPHY WITH A MULTI-WIRE PROPORTIONAL
CHAMBER--A STATUS REPORT*

Summary

Previously reported prototype studies^{1,2} have been extended through the construction of a 25 cm × 25 cm neutron-sensitive multi-wire proportional chamber. The basic chamber consists of three parallel wire-grid planes in a gas-filled envelope. The central, anode plane consists of a parallel array of 13 μm-diameter gold-plated tungsten wires separated from each other by 1.5 mm but terminating electrically in common on an outer frame. The outer, cathode grids consist of 37 μm-diameter wires separated from each other by 1 mm. The two outermost grid planes have their wire axes mutually orthogonal. The proportional gas used was 93% Ar and 7% methane. The inner faces of the chamber windows are coated with ¹⁰B to achieve neutron sensitivity. A signal that indicates the occurrence of an ionizing event in the chamber is obtained from the central plane. The two outer grids provide the spatial information. Each wire of the orthogonal outer planes is coupled capacitively to an electromagnetic delay line. The time interval between the occurrence of the central grid signal and the delayed cathode signal determines the location of the event in each of two orthogonal directions. This information may either be digitally encoded for computer storage or converted, by means of time-to-amplitude converters into x-y deflection pulses for an oscilloscope display. (A more complete design description may be found in Ref. 2.) An example of such an oscilloscope-displayed image is compared with a high-resolution Gd-screen photographic image in Fig. 1. The single B conversion screen converter used for obtaining this image was made simply by embedding

powdered ^{10}B (92% enriched) in double-sided masking tape placed on the inside face of one of the chamber windows. The converter made in this manner caused no observed electrical problems, had a mean thickness of 4 mgm-cm^{-2} , and gave a measured useful converter efficiency of 2%. The resolution characteristics of this larger chamber are approximately the same as those of the small prototype previously described.^{1,2} Improvements in converter construction as well as the addition of a second converter are expected to increase the efficiency to a value closer to the calculated 7%. Increasing the gas density, either by pressurizing the chamber or by using a heavier gas such as xenon, is expected to improve resolution by shortening the alpha-particle track lengths.

Figure Caption


Fig. 1. Neutron radiographs of an aluminum-cased electric drill. (The screw in the drill chuck is made from nylon.)

(a) High resolution film-type neutron radiograph requiring approximately 10^{10} n/cm^2 .

(b) Wire-chamber image as produced by a succession of points displayed on a conventional oscilloscope. Note that the wire chamber image while not showing fine details such as the threads on the nylon screw nor the features of the brush housing can show larger features such as the grease in the gear box and the plastic components of the trigger mechanism. The wire chamber image required 10^{-5} the flux of the photographic image and corresponds to 20 detected neutrons per square millimeter. An image of $1\text{-}2$ n-mm^{-2} shows essentially all of the same features but has a more grainy appearance.


Footnote and References

- * Work done under the auspices of the U. S. Atomic Energy Commission.
1. S. KAPLAN, K. VALENTINE, LEON KAUFMAN, and V. PEREZ MENDEZ, Neutron Radiography With a Multi-Wire Proportional Chamber - Performance and Projections, Trans. Am. Nucl. Soc. 13, 140 (1972).
 2. S. KAPLAN, L. KAUFMAN, V. PEREZ MENDEZ, and K. VALENTINE, Multi-Wire Proportional Chambers for Biomedical Application, Nucl. Instr. Methods, in press.

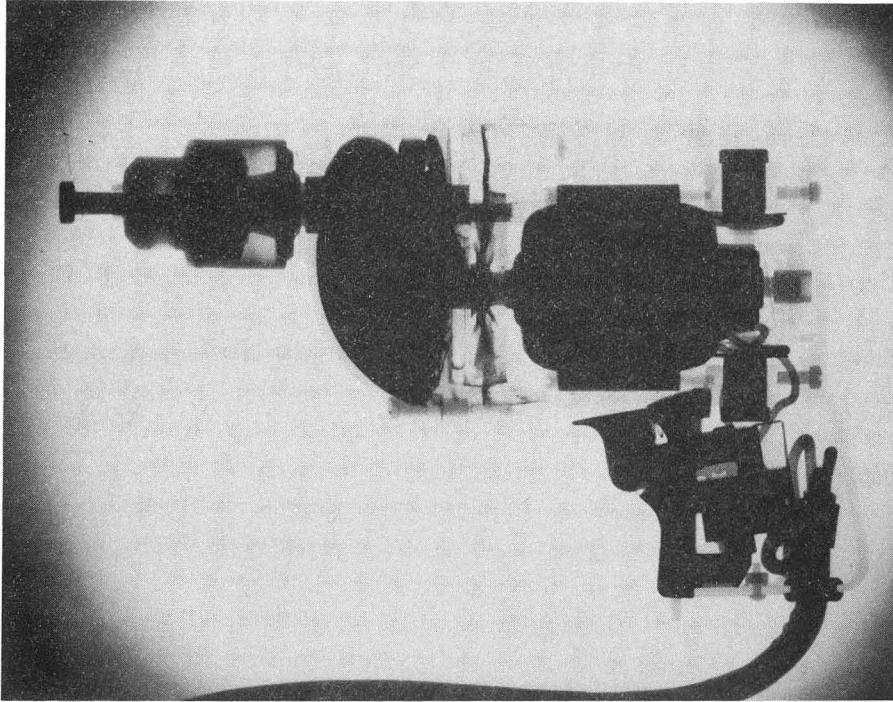

(a)

XBB 728-3848

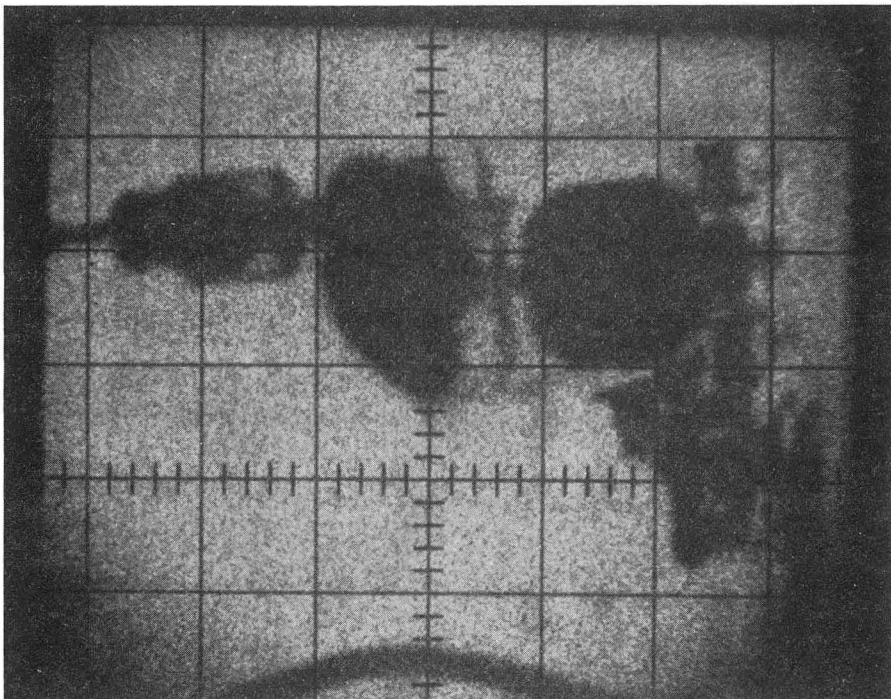

(b)

XBB 728-3847A

Fig. 1

LEGAL NOTICE

This report was prepared as an account of work sponsored by the United States Government. Neither the United States nor the United States Atomic Energy Commission, nor any of their employees, nor any of their contractors, subcontractors, or their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness or usefulness of any information, apparatus, product or process disclosed, or represents that its use would not infringe privately owned rights.

TECHNICAL INFORMATION DIVISION
LAWRENCE BERKELEY LABORATORY
UNIVERSITY OF CALIFORNIA
BERKELEY, CALIFORNIA 94720