

UCLA

UCLA Previously Published Works

Title

Effectiveness of N95 Respirator Decontamination and Reuse against SARS-CoV-2 Virus.

Permalink

<https://escholarship.org/uc/item/1773m663>

Journal

Emerging Infectious Diseases, 26(9)

Authors

van Doremalen, Neeltje
Sarchette, Shanda
Matson, M
[et al.](#)

Publication Date

2020-09-01

DOI

10.3201/eid2609.201524

Peer reviewed

About the Author

Dr. Leshem is a clinical associate professor at Tel Aviv University School of Medicine and the director of the Institute for Travel Medicine and Tropical Diseases at Sheba Medical Center in Tel Hashomer, Israel. His research interests include global health, epidemiology, and vaccine-preventable diseases.

References

1. Israel Central Bureau of Statistics. Population of Israel on the eve of 2020. 2019 [cited 2020 Mar 25]. <https://www.cbs.gov.il/en/mediarelease/Pages/2019/Population-of-Israel-on-the-Eve-of-2020.aspx>
2. Organization for Economic Cooperation and Development. OECD data: hospital beds. 2020 [cited 2020 Mar 22]. <https://data.oecd.org/healthqt/hospital-beds.htm>
3. State of Israel Ministry of Health. Hospitalization beds in Israel, January 2020 [in Hebrew]. 2020 [cited 2020 Apr 12]. https://www.health.gov.il/UnitsOffice/HD/MTI/info/Pages/licensed_inpatient_hospital_beds.aspx
4. State of Israel Ministry of Health Information Division. Hospital occupancy by admission ward and month, 2016–2017 [in Hebrew]. 2017 [cited 2020 Mar 25]. https://www.health.gov.il/UnitsOffice/HD/MTI/info/Pages/hospital_Beds.aspx
5. Chernichovsky D. Not “socialized medicine” – an Israeli view of health care reform. *N Engl J Med*. 2009;361:e46. <https://doi.org/10.1056/NEJMp0908269>
6. Israel Central Bureau of Statistics. Israel visitor arrivals in January–November 2019 [in Hebrew]. 2020 [cited 2020 Mar 25]. https://www.cbs.gov.il/he/mediarelease/DocLib/2019/367/28_19_367b.pdf
7. State of Israel Ministry of Health. HaMagen: the Ministry of Health app for fighting the COVID-19 outbreak. 2020 [cited 2020 May 12]. <https://govextra.gov.il/ministry-of-health/hamagen-app/download-en>
8. State of Israel Ministry of Health. A general statement of illness for isolated workers. 2020 [cited 2020 May 12]. <https://govextra.gov.il/ministry-of-health/corona/corona-virus-en>
9. State of Israel Ministry of Health. COVID-19 resources [in Hebrew]. 2020 [cited 2020 May 12]. <https://data.gov.il/dataset/covid-19/<eref>>
10. Leshem E, Klein Y, Haviv Y, Berkenstadt H, Pessach IM. Enhancing intensive care capacity: COVID-19 experience from a tertiary center in Israel. *Intensive Care Med*. 2020 May 25 [Epub ahead of print]. PubMed <https://doi.org/10.1007/s00134-020-06097-0>

Address for correspondence: Eyal Leshem, Institute for Travel Medicine and Tropical Diseases, Sheba Medical Center, Tel Hashomer 52621, Israel; email: Eyal.Leshem@sheba.health.gov.il

Effectiveness of N95 Respirator Decontamination and Reuse against SARS-CoV-2 Virus

Robert J. Fischer, Dylan H. Morris, Neeltje van Doremalen, Shanda Sarchette, M. Jeremiah Matson, Trenton Bushmaker, Claude Kwe Yinda, Stephanie N. Seifert, Amandine Gamble, Brandi N. Williamson, Seth D. Judson, Emmie de Wit, James O. Lloyd-Smith, Vincent J. Munster

Author affiliations: National Institute of Allergy and Infectious Diseases, Hamilton, Montana, USA (R.J. Fischer, N. van Doremalen, S. Sarchette, M.J. Matson, T. Bushmaker, C.K. Yinda, S.N. Seifert, B.N. Williamson, E. de Wit, V.J. Munster); Princeton University, Princeton, New Jersey, USA (D.H. Morris); Marshall University, Huntington, West Virginia, USA (M.J. Matson); University of California, Los Angeles, Los Angeles, California, USA (A. Gamble, J.O. Lloyd-Smith), University of Washington, Seattle, Washington, USA (S.D. Judson)

DOI: <https://doi.org/10.3201/eid2609.201524>

The coronavirus pandemic has created worldwide shortages of N95 respirators. We analyzed 4 decontamination methods for effectiveness in deactivating severe acute respiratory syndrome coronavirus 2 virus and effect on respirator function. Our results indicate that N95 respirators can be decontaminated and reused, but the integrity of respirator fit and seal must be maintained.

The unprecedented pandemic of coronavirus disease has created worldwide shortages of personal protective equipment, in particular respiratory protection such as N95 respirators (1). Transmission of severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) occurs frequently in hospital settings; numerous reported cases of nosocomial transmission highlight the vulnerability of healthcare workers (2). The environmental stability of SARS-CoV-2 virus underscores the need for rapid and effective decontamination methods.

In general, N95 respirators are designed for one use before disposal. Extensive literature is available for decontaminating N95 respirators, of either bacterial spores, bacteria, or respiratory viruses (e.g. influenza A virus) (3–6). Effective inactivation methods for these pathogens and surrogates include UV light, ethylene oxide, vaporized hydrogen peroxide (VHP), gamma irradiation, ozone, and dry heat (A. Cramer et al., unpub data, <https://doi.org/10.1101/2020.03.28.20043471>) (3–6). The filtration efficiency and fit of N95 respirators has been less well explored, but reports

suggest that both filtration efficiency and N95 respirator fit can be affected by the decontamination method used (7; Appendix, <https://wwwnc.cdc.gov/EID/article/26/9/20-1524-App1.pdf>).

We analyzed 4 different decontamination methods, UV light (260–285 nm), 70°C dry heat, 70% ethanol, and VHP, for their ability to reduce contamination with infectious SARS-CoV-2 and their effect on N95 respirator function. The starting inoculum of SARS-CoV-2 has cycle threshold values of 20–22, similar to those observed in samples obtained from the upper and lower respiratory tract in humans. For

each of the decontamination methods, we compared the normal inactivation rate of SARS-CoV-2 virus on N95 filter fabric to that on stainless steel. Using quantitative fit testing, we measured the filtration performance of N95 respirators after each decontamination run and 2 hours of wear, for 3 consecutive decontamination and wear sessions (Appendix). VHP and ethanol yielded extremely rapid inactivation both on N95 and on stainless steel (Figure, panel A). UV light inactivated SARS-CoV-2 virus rapidly from steel but more slowly on N95 fabric, probable because of its porous nature. Heat caused more rapid inactivation

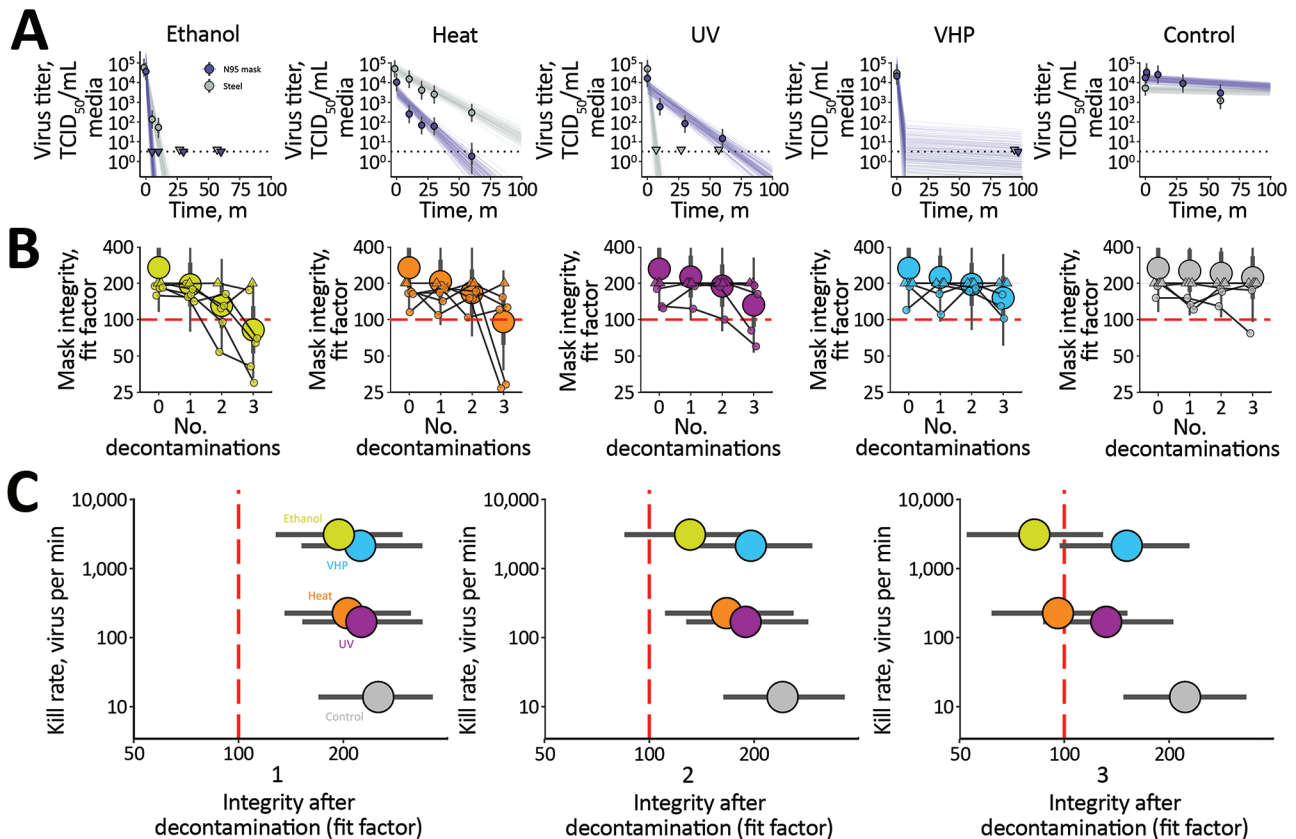


Figure. Results of decontamination of N95 respirators by 4 different methods. A) Inactivation of severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) virus (Appendix, <https://wwwnc.cdc.gov/EID/article/26/9/20-1524-App1.pdf>). Points indicate estimated mean viable titer across 3 replicates, circles the posterior median estimate of the mean, thick bars a 68% credible interval, and thin bars a 95% credible interval. Lines show predicted decay of virus titer over time and were generated by 50 random draws/replicate from the joint posterior distribution of the exponential decay rate (negative of the slope) and intercept (initial virus titer). Time points with no positive wells for any replicate are plotted as triangles at the approximate single-replicate LOD to indicate a plausible range of sub-LOD values. Black dotted line shows approximate LOD: $10^{0.5}$ TCID₅₀/mL media. Points at the LOD and at $t = 0$ for ethanol and heat methods applied to steel are offset slightly up and to the left to avoid overplotting. B) Mask integrity quantitative fit testing results after decontamination and 2 hours of wear for 3 consecutive runs. Data from 6 individual replicates (small circles and triangles) for each treatment are shown, in addition to estimated median fit factor (large circles), 68% range of underlying fit factors (thick bars), and 95% range (thin bars). Fit factors are a measure of filtration performance, the ratio of the concentration of particles outside the mask to the concentration inside. The measurement machine reports values ≤ 200 ; measured values of 200 are shown as upward-pointing triangles to indicate that true underlying values may be higher; other measured values are shown as circles. A minimal fit factor of 100 (red dashed line) is required for a mask to pass a fit test. See also Appendix Figure 3. C) SARS-CoV-2 decontamination performance after 1, 2, and 3 decontamination cycles, shown as kill rate vs. mask integrity after decontamination. Circles represent estimated median, bar length estimated 68% range. LOD, limit of detection; TCID₅₀, 50% tissue culture infective dose; VHP, vaporized hydrogen peroxide.

on N95 than on steel; inactivation rates on N95 were comparable to UV.

Quantitative fit tests showed that the filtration performance of the N95 respirator was not markedly reduced after a single decontamination for any of the 4 decontamination methods (Figure, panel B). Subsequent rounds of decontamination caused sharp drops in filtration performance of the ethanol-treated masks and, to a slightly lesser degree, the heat-treated masks. The VHP- and UV-treated masks retained comparable filtration performance to the control group after 2 rounds of decontamination and maintained acceptable performance after 3 rounds.

Our findings showed that VHP treatment had the best combination of rapid inactivation of SARS-CoV-2 virus and preservation of N95 respirator integrity under the experimental conditions (Figure, panel C). UV light killed the virus more slowly and preserved respirator function almost as well. Dry heat at 70°C killed the virus with similar speed to UV and is likely to maintain acceptable fit scores for 1–2 rounds of decontamination but should not be used for 3 rounds. Consistent with earlier findings (8), ethanol decontamination reduced N95 integrity and is not recommended.

All treatments, particularly UV light and dry heat, should be conducted for long enough to ensure sufficient reduction in virus concentration. The degree of required reduction depends upon the degree of initial virus contamination. Policymakers can use our estimated decay rates together with estimates of real-world contamination to choose appropriate treatment durations (Appendix).

Our results indicate that, in times of shortage, N95 respirators can be decontaminated and reused up to 3 times by using UV light and HPV and 1–2 times by using dry heat. Following nationally established guidelines for fit testing, seal check, and respirator reuse is critical (9,10). We recommend performing decontamination for sufficient time and ensuring proper function of the respirators after decontamination using readily available qualitative fit testing tools.

Acknowledgments

We thank Madison Hebner, Julia Port, Kimberly Meade-White, Irene Offei Owusu, Victoria Avanzato, and Lizzette Perez-Perez for excellent technical assistance.

This research was supported by the Intramural Research Program of the National Institute of Allergy and Infectious Diseases, National Institutes of Health. J.O.L.-S. and A.G. were supported by the Defense Advanced Research Projects Agency PREEMPT no. D18AC00031 and the UCLA AIDS Institute and Charity Treks, and J.O.L.-S. was supported

by the US National Science Foundation (DEB-1557022), the Strategic Environmental Research and Development Program (RC-2635) of the US Department of Defense.

About the Author

Dr. Fischer is a member of the Virus Ecology Section at the Rocky Mountain Laboratories Division of Intramural Research, National Institute of Allergy and Infectious Diseases, National Institutes of Health. His research interests include the ecology of emerging viruses in their natural and spillover hosts, including SARS-CoV-2.

References

1. Ranney ML, Griffeth V, Jha AK. Critical supply shortages— the need for ventilators and personal protective equipment during the Covid-19 pandemic. *N Engl J Med*. 2020;382:e41. <https://doi.org/10.1056/NEJMp2006141>
2. McMichael TM, Currie DW, Clark S, Pogosjans S, Kay M, Schwartz NG, et al. Epidemiology of Covid-19 in a long-term care facility in King County, Washington. *N Engl J Med*. 2020; [NEJMoa2005412](https://doi.org/10.1056/NEJMoa2005412). <https://doi.org/10.1056/NEJMoa2005412>
3. Batelle. Final report for the Bioquell hydrogen peroxide vapor (HPV) decontamination for reuse of N95 respirators. 2016 [cited 2020 May 22]. <https://www.fda.gov/media/136386/download>
4. Fisher EM, Shaffer RE. A method to determine the available UV-C dose for the decontamination of filtering facepiece respirators. *J Appl Microbiol*. 2011;110:287–95. <https://doi.org/10.1111/j.1365-2672.2010.04881.x>
5. Heimbuch BK, Wallace WH, Kinney K, Lumley AE, Wu CY, Woo MH, et al. A pandemic influenza preparedness study: use of energetic methods to decontaminate filtering facepiece respirators contaminated with H1N1 aerosols and droplets. *Am J Infect Control*. 2011;39:e1–9. <https://doi.org/10.1016/j.ajic.2010.07.004>
6. Lin TH, Tang FC, Hung PC, Hua ZC, Lai CY. Relative survival of *Bacillus subtilis* spores loaded on filtering facepiece respirators after five decontamination methods. *Indoor Air*. 2018;28:754–62. <https://doi.org/10.1111/ina.12475>
7. Lin TH, Chen CC, Huang SH, Kuo CW, Lai CY, Lin WY. Filter quality of electret masks in filtering 14.6–594 nm aerosol particles: effects of five decontamination methods. *PLoS One*. 2017; [12:e0186217](https://doi.org/10.1371/journal.pone.0186217). <https://doi.org/10.1371/journal.pone.0186217>
8. Viscusi DJ, Bergman MS, Eimer BC, Shaffer RE. Evaluation of five decontamination methods for filtering facepiece respirators. *Ann Occup Hyg*. 2009;53:815–827. <https://doi.org/10.1093/annhyg/mep070>
9. US Centers for Disease Control and Prevention. Decontamination and reuse of filtering facepiece respirators. 2020 [cited 2020 Apr 5]. <https://www.cdc.gov/coronavirus/2019-ncov/hcp/ppe-strategy/decontamination-reuse-respirators.html>
10. US National Institute for Occupational Safety and Health; US Centers for Disease Control and Prevention. Recommended guidance for extended use and limited reuse of N95 filtering facepiece respirators in healthcare settings. 2020 [cited 2020 May 22]. <https://www.cdc.gov/niosh/topics/hcwcontrols/recommendedguidanceextuse.html>

Address for correspondence: Vincent Munster, NIAID/NIH, Laboratory of Virology, Rocky Mountain Laboratories, 9035 4th St, Hamilton, MT 59840, USA; email: vincent.munster@nih.gov