

UC San Diego

UC San Diego Previously Published Works

Title

Aseptic Stethoscope Barriers Prevent C difficile Transmission In Vitro

Permalink

<https://escholarship.org/uc/item/22p3h4hr>

Journal

Mayo Clinic Proceedings Innovations Quality & Outcomes, 5(1)

ISSN

2542-4548

Authors

Peacock, W Frank
Kalra, Sarathi
Vasudevan, Rajiv S
[et al.](#)

Publication Date

2021-02-01

DOI

10.1016/j.mayocpiqo.2020.10.002

Copyright Information

This work is made available under the terms of a Creative Commons Attribution-NonCommercial-NoDerivatives License, available at <https://creativecommons.org/licenses/by-nc-nd/4.0/>

Peer reviewed

Aseptic Stethoscope Barriers Prevent *C difficile* Transmission In Vitro

W. Frank Peacock, MD; Sarathi Kalra, MD; Rajiv S. Vasudevan;
and Francesca Torriani, MD

Abstract

Objective: To evaluate whether *Clostridioides* (formerly *Clostridium*) *difficile*—contaminated stethoscope diaphragms remained aseptic by the placement of an aseptic diaphragm barrier.

Methods: On November 1, 2019, fresh cultures of *C difficile* were diluted to 10^7 colony-forming units (CFU)/mL and used to inoculate 16 stethoscope diaphragms; 8 had an aseptic diaphragm barrier applied and 8 served as nonbarrier controls. Contaminated stethoscopes were anaerobically incubated, then swabbed at 15 and 30 minutes, 2 and 4 hours, and 1, 2, 3, and 7 days after inoculation and subsequently plated onto blood, chocolate, and cycloserine-cefoxitin fructose agar. Plates were incubated for 48 hours and on November 9, 2019, the resulting colonies were manually counted. Statistical analyses (RStudio, version 1.0.153) used analysis of variance with post hoc Tukey honestly significant difference.

Results: Overall, mean colony count was 33 CFU on stethoscopes without barriers vs zero on those with barriers ($P \leq .05$). Growth was greatest at 48 hours, with colony counts as high as 160 CFU. The presence of the barrier resulted in no growth in 100% of stethoscope diaphragms for up to 1 week.

Conclusion: We found that stethoscope diaphragm barriers provide an aseptic patient contact point, thus reducing the potential for transmission of *C difficile* during the physical examination. In critical care environments, in which many hospitals use acoustically inferior disposable stethoscopes, the option of a disposable aseptic stethoscope barrier may allow high-quality auscultation while reducing the potential for pathogen transmission.

© 2020 THE AUTHORS. Published by Elsevier Inc on behalf of Mayo Foundation for Medical Education and Research. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>) ■ Mayo Clin Proc Inn Qual Out 2021;5(1):103-108

Clostridioides (formerly *Clostridium*) *difficile* infection (CDI) is a major public health issue. *Clostridioides difficile* is an anaerobic gram-positive bacteria that can generate infection-causing spores that are highly resistant to heat and alcohol disinfectants. Infection commonly occurs following fecal-oral transmission of spores in patients taking systemic broad-spectrum antibiotics, which disrupt healthy gut flora and allow *C difficile* proliferation. Although guideline-compliant handwashing may limit *C difficile* transmission, alcohol-based hand rubs may be ineffective for removing spores from hands.¹ The persistence of *C difficile* spores in hospital environments has led to a high prevalence of CDI. In 2015, there were an estimated 450,000 US CDI cases, which resulted in 35,000 deaths.² Although overall rates of CDI have stabilized, rates of recurrent CDI,

defined as greater than 1 recurrence after an initial CDI, have increased from 1.1 to 3.1 cases per 100,000 person-years from 2001 to 2012.³ Because CDI and recurrent CDI are associated with severe adverse outcomes, novel strategies to prevent iatrogenic and nosocomial spread would be invaluable.

One potential source of iatrogenic CDI may be the stethoscope. An important interface during the patient examination, the stethoscope is used to examine most hospitalized patients. The Centers for Disease Control and Prevention guidelines define the stethoscope as a noncritical medical device (ie, in contact with intact skin but not bodily fluids) and recommend cleaning for longer than 1 minute after each patient interaction using an alcohol- or bleach-based disinfectant.⁴ Unfortunately, recent studies demonstrate dismal rates of stethoscope hygiene compliance in

From the Department of Emergency Medicine, Baylor College of Medicine, Houston, TX (W.F.P.); Department of Emergency Medicine, University of South Alabama, AL (S.K.); and Department of Medicine, University of California San Diego School of Medicine, San Diego, CA (R.S.V., F.T.).

the clinical setting, with observed cleaning rates occurring in less than 10% of patient encounters.⁵⁻¹²

Despite most providers understanding that the unsanitized stethoscope may be a microbial transmission vector,¹³ poor stethoscope hygiene rates are persistent. When questioned, providers report barriers to hygiene performance that include the lack of time and poor access to disinfectants. Contributing to the potential of nosocomial infection, the recent literature questions the ability of common disinfectants to completely eliminate contaminating bacteria.¹⁴ In 1 study, *Enterococcus faecium* was demonstrated to have an increasing tolerance to 70% isopropyl alcohol solutions,¹⁵ which may result in its continued presence on the stethoscope even if it is cleaned per guideline recommendations. Coupled with the resistance of *C difficile* spores to alcohol-based disinfectants, this emerging evidence highlights the critical need for alternatives to alcohol- or bleach-based stethoscope cleaning processes.

Aseptic stethoscope barriers have been suggested as a more time-efficient and bacteriologically effective method to ensure a clean interface between the patient and the stethoscope diaphragm.¹¹ The purpose of this study was to evaluate the ability of a single-use aseptic barrier to prevent the transmission of *C difficile* from a stethoscope diaphragm.

This study was approved by the University of California, San Diego Administrative Panel on Human Subjects in Medical Research and was certified as category 4 exempt, which does not require informed consent.


METHODS

This was an experimental study evaluating the effectiveness of a barrier to prevent the transmission of *C difficile* from a contaminated stethoscope diaphragm. Specimens of *C difficile* were obtained from ATCC, Inc. On November 1, 2019, two replicate clinical strains of *C difficile* were prepared. Fresh cultures of *C difficile* were diluted to 10^7 colony-forming units (CFU)/mL, and using Copan FLOQswabs (Copan Diagnostics Inc), were dipped into the vortexed diluted cultures. Inoculation of 16 stethoscope diaphragms was then performed (Figure 1). After the diaphragms were allowed to dry for 10 minutes, 8 stethoscopes had a

barrier (Aseptiscope Inc) placed on the diaphragm, whereas the remaining 8 stethoscopes, serving as controls, had no barrier placed. The barrier was obtained from a hands-free dispenser system that provides a safe, medical-grade, impervious, aseptic, single-use disposable biocompatible tape that is acoustically invisible and leaves no residue on the stethoscope after removal. The stethoscopes were then placed in an anaerobic incubator and at the prespecified times of 15 and 30 minutes, 2 and 4 hours, and 1, 2, 3, and 7 days, the diaphragms of the control stethoscopes and the barriers of the interventional stethoscopes were swabbed with a clean swab, which was then placed into Eswab media (Becton-Dickinson). Subsequently, cultures were plated onto blood, chocolate, and cycloserine-cefoxitin fructose agar plates using the Copan WASP automated planting system (Copan Diagnostics Inc). These plates were incubated for 48 hours anaerobically using an Anoxomat Mark II System (Advanced Instruments Inc), and any resulting colonies were manually counted on November 9, 2019.

Statistical Analyses

Statistical analyses were performed using RStudio, version 1.0.153 (R Studio).

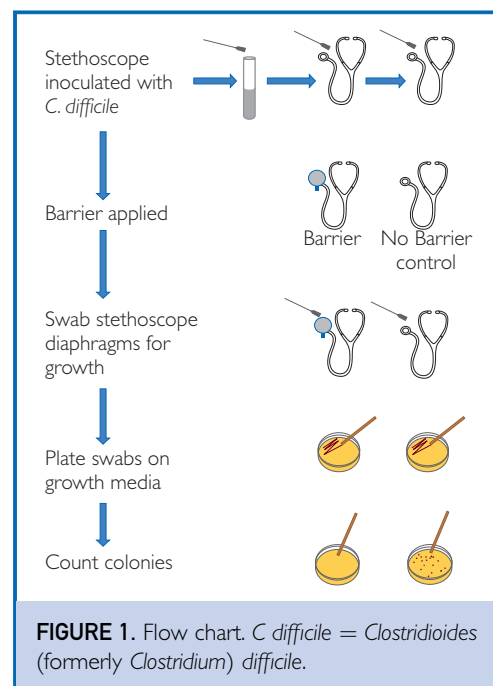

Differences in colony counts between stethoscope diaphragms with and without barriers were determined using 1-tailed *t* tests. To compare colony counts from stethoscope diaphragms with barriers vs those without barriers, analysis of variance with post hoc Tukey honestly significant difference tests were used.


RESULTS

In this longitudinal assessment of *C difficile* growth on the stethoscope diaphragms without aseptic barriers, we reliably detected *C difficile* at all time points. Overall, the mean colony count was 33 CFU on the 8 stethoscopes without barriers (Figure 2). Growth rates were greatest at 48 hours, with colony counts as high as 160 CFU (Figure 3). Culturing the barrier surface of the *C difficile*-contaminated stethoscope diaphragm after incubation yielded no *C difficile* regardless of the time of exposure to *C difficile*. Colony counts were zero on all stethoscope diaphragms covered with barriers. The *C difficile* growth findings on stethoscope diaphragms without barriers were in stark contrast to those with barriers in respect to *C difficile* culture growth. The presence of the barrier resulted in no growth from 100% of stethoscope diaphragms for up to 1 week after contamination.

The difference in colony counts was evaluated using a 1-tailed *t* test. At each time point, there was a significant ($P < .05$) absence of *C difficile* growth on the stethoscope diaphragms with the barriers compared with growth on diaphragms without barriers. Although the stethoscope diaphragm is not be the only source of *C difficile* transmission, these results suggest that aseptic barriers will prevent transmission of *C difficile* bacteria from a contaminated stethoscope diaphragm to a patient.

DISCUSSION

We tested the ability of aseptic barriers to prevent an unwashed *C difficile*-contaminated stethoscope diaphragm from serving as an iatrogenic vector between patients. Our results suggest that a stethoscope diaphragm that is contaminated with *C difficile* is rendered aseptic by the placement of a bacteriologically impervious barrier. Although we focused on *C difficile* as the primary agent, prior work supports the concept that an impervious barrier

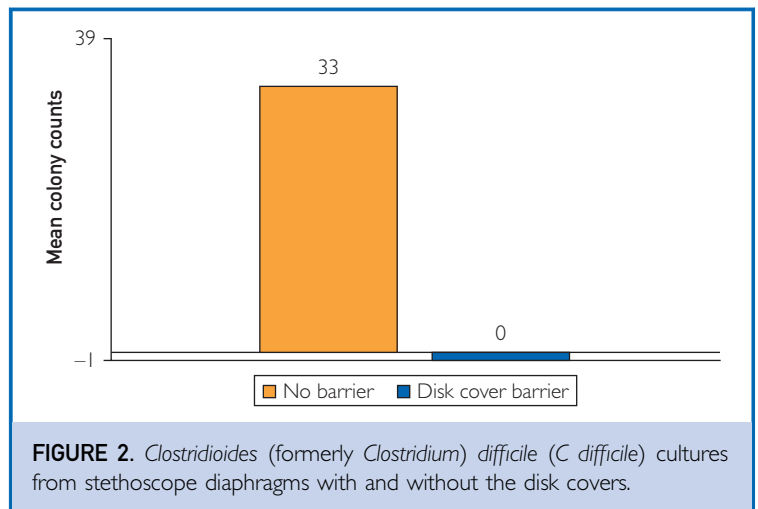

is efficacious in preventing the stethoscope diaphragm from becoming an infectious vector. In one study by Vasudevan et al,¹¹ aseptic barriers placed on the stethoscope diaphragm that had been contaminated with anaerobes, antibiotic-resistant bacteria, yeasts, and infected samples that included saliva, stool, urine, and sputum were persistently sterile for up to 24 hours. Further, studies evaluating stethoscope diaphragms contaminated with vancomycin-resistant *Enterococcus* (VRE), methicillin-resistant *Staphylococcus aureus*; extended-spectrum β -lactamase-producing *Escherichia coli*; and multidrug resistant *Pseudomonas aeruginosa*, *Staphylococcus epidermidis*, *Bacteroides* species, and *Candida albicans* have demonstrated the same results.¹¹ Considering these prior studies, as well as the findings from our investigation, it is clear that a cover placed over the stethoscope diaphragm can provide an aseptic point of patient contact.

As hospitals have recognized the importance of stethoscope hygiene for infection prevention practice,¹⁶ many institutions have attempted to provide alternatives to the contaminated stethoscope. Unfortunately, this has not elicited effective results. Education seems to have a poor effect in changing health care provider stethoscope cleaning behavior. One investigation provided stethoscope hygiene visual reminders and alcohol swab-containing baskets on the hospital wards. They reported stethoscope hygiene rates no higher than 59%.¹⁷ Another

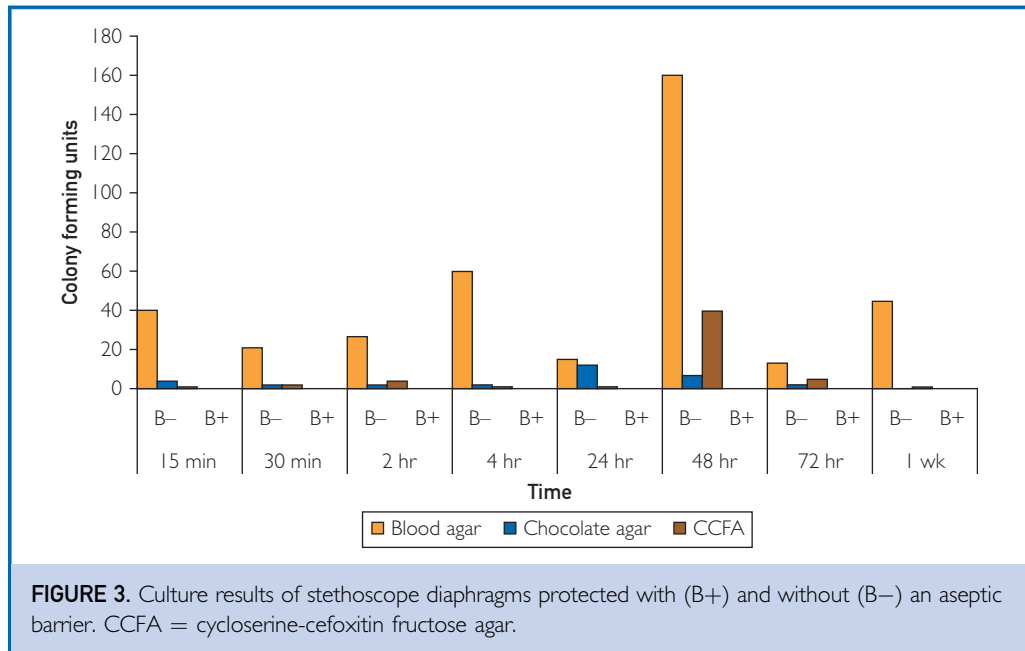


FIGURE 3. Culture results of stethoscope diaphragms protected with (B+) and without (B-) an aseptic barrier. CCFA = cycloserine-cefoxitin fructose agar.

intervention implementing a similar protocol with the addition of providing informational lectures to the medical staff observed absolutely no compliance (0%) either before or after the intervention.¹⁸ It seems well documented that education has limited effectiveness at improving stethoscope hygiene, a result that suggests that alternative interventions are necessary to prevent a stethoscope vector from contaminating patients.

Strategies that are commonly used, especially for patients infected with multidrug-resistant organisms (MDROs), include the implementation of contact precautions, strict hand washing protocols, and the use of disposable gowns, gloves, and single-patient disposable stethoscopes to decrease the likelihood of transfer to other patients.¹⁹ Although effective for infection control,²⁰ the single-patient disposable stethoscope allows only suboptimal auscultation due to poor audio quality,²¹ potentially leading health care providers to abandon their use in favor of their own stethoscopes. This not only results in the potential contamination of the provider's stethoscope with an MDRO, but also creates the exact scenario that the disposable stethoscope was implemented to prevent; that is,

facilitating the transfer of an MDRO to other hospitalized patients.²²

A simple answer to the challenge of the contaminated stethoscope could be the requirement of stethoscope disinfection. Unfortunately, data regarding this strategy have not been reassuring. In a self-reported survey study of 1401 physicians, 76% believed stethoscope hygiene to be important but only 24% reported cleaning their stethoscope regularly.¹³ Observational studies suggest that the reported rate is actually inflated. Jenkins et al²³ reported that in 352 stethoscope cleaning opportunities, physicians or students cleaned their stethoscope in only 16% of encounters (n=58). Even worse rates were reported by Boulee et al,²⁴ who noted that in 84 patient encounters, only 4% of attending physicians cleaned their stethoscopes in a guideline-compliant fashion. Ultimately, although health care professionals recognize the importance of stethoscope hygiene, it is rarely performed.

Finally, even when the stethoscope is disinfected, complete sterility may not result. Zachary et al²⁵ found that 31% of stethoscopes are contaminated with VRE and although washing with 70% alcohol decreases VRE contamination, an absolute 2% of

stethoscopes remain VRE positive. Similarly, Parmar et al²⁶ cultured 100 health care worker's stethoscopes, finding that 90% are positive for some staphylococcus species, and after washing with 66% isopropyl alcohol, 28% remain culture positive. These studies suggest that even guideline-compliant stethoscope washing does not guarantee sterility.

The most concerning investigation of a stethoscope washing strategy is recent research published by Pidot et al.¹⁵ They report that from 1997 to 2015, *E faecium* tolerance to 70% alcohol has increased 10-fold. This suggests that the Centers for Disease Control and Prevention recommendation that the stethoscope be cleaned for 1 minute with 70% alcohol swabs between patients may become ineffective in the future.

As we report, medical-grade aseptic barriers that do not affect the subjective quality of auscultation²⁷ can provide physical protection from microbes. Ideally, these single-use barriers are applied to the stethoscope diaphragm from a hands-free dispenser just before evaluating the patient, thus ensuring hygienic patient contact similar to that obtained by disposable gowns/gloves. The potential benefits of barriers include reduced transmission of pathogenic and antibiotic-resistant microbes, as well as the improved quality of auscultation by the use of the physician's clean personal stethoscope rather than that of the single-patient disposable stethoscopes.²¹

Alternatively, other stethoscope hygiene solutions have been described. One study evaluated the antimicrobial properties of a copper-alloy metal stethoscope, citing decreased levels of contamination. However, it did not mention the cost of implementing such a change.²⁸ Another investigated a stethoscope UV light case but reported incomplete decontamination.²⁹ An additional study investigated an antimicrobial stethoscope coating,³⁰ but such a coating could select for resistant microorganisms. Our study demonstrated the effectiveness of an aseptic diaphragm barrier without antimicrobial properties (Figure 3) to limit the formation and propagation of resistant pathogens. Because the barriers are disposable, are single-use, and work by providing a physical rather than antimicrobial barrier, they provide

protection without the risk for resistant microorganisms. Although prior technologies have accomplished only a partial reduction in stethoscope contamination, our data support that diaphragm barriers are capable of remaining aseptic against pathogens.

This study has some limitations. This was a small in vitro evaluation of *C difficile* placed on stethoscope diaphragms and did not evaluate the potential for human-to-human infection. It is possible that in vivo evaluations could show different viability rates. However, our rates suggest that *C difficile* can survive on the unprotected stethoscope diaphragm, which should be of concern to both patients and practitioners. Furthermore, real-life studies could identify other relevant contact points for *C difficile* transmission, such as the examiner's hands and stethoscope tubing. Finally, costs were not examined in this evaluation. The relevant expense of disposable stethoscopes (eg, dollars) vs disposable barriers (eg, cents) could have important infection control decision-making attributes.

CONCLUSION

We found that stethoscope diaphragm barriers provide an aseptic patient contact point, thus reducing the potential for transmission of *C difficile* during the physical examination. In critical care environments, in which many hospitals use acoustically inferior disposable stethoscopes, the option of a disposable aseptic stethoscope barrier may allow high-quality auscultation while reducing the potential for pathogen transmission.



Abbreviations and Acronyms: **CCFA** = cycloserine-cefoxitin fructose agar; **CDI** = *Clostridioides* (formerly *Clostridium*) *difficile* infection; **CFU** = colony-forming unit; **MDRO** = multidrug resistant organism; **VRE** = vancomycin-resistant *Enterococcus*

Grant Support: This study was supported by an unrestricted grant to the University of California, San Diego by Aseptiscope, Inc (San Diego, CA). No author received funding for the performance of this study.

Potential Competing Interests: Dr Peacock holds stock in Aseptiscope, Inc. The remaining authors report no competing interests.

Correspondence: Address to W. Frank Peacock, MD, Ben Taub General Hospital, Emergency Department, 1504 Taub Loop, Houston, TX 77030 (frankpeacock@gmail.com).

ORCID

W. Frank Peacock:  <https://orcid.org/0000-0002-2730-6742>; Sarathi Kalra:  <https://orcid.org/0000-0002-5619-3396>; Rajiv S. Vasudevan:  <https://orcid.org/0000-0003-0935-0456>

REFERENCES

- Jabbar U, Leischner J, Kasper D, et al. Effectiveness of alcohol-based hand rubs for removal of *Clostridium difficile* spores from hands. *Infect Control Hosp Epidemiol*. 2010;31(6):565-570.
- Lessa FC, Mu Y, Bamberg WM, et al. Burden of *Clostridium difficile* infection in the United States. *N Engl J Med*. 2015;372(9):825-834.
- Ma GK, Brensinger CM, Wu Q, Lewis JD. Increasing incidence of multiply recurrent *Clostridium difficile* infection in the United States: a cohort study. *Ann Intern Med*. 2017;167(3):152-158.
- Rutala WA, Weber DJ, Healthcare Infection Control Practices Advisory Committee (HICPAC) Guideline for Disinfection and Sterilization in Healthcare Facilities, 2008 Update. Centers for Disease Control and Prevention; 2017. <https://www.cdc.gov/infectioncontrol/guidelines/disinfection/>. [Accessed 16124 November 2020]
- Fenelon L, Holcroft L, Waters N. Contamination of stethoscopes with MRSA and current disinfection practices. *J Hosp Infect*. 2009;71(4):376-378.
- Jones JS, Hoerle D, Riekse R. Stethoscopes: a potential vector of infection? *Ann Emerg Med*. 1995;26(3):296-299.
- Madar R, Novakova E, Baska T. The role of non-critical healthcare tools in the transmission of nosocomial infections. *Bratisl Lek Listy*. 2005;106(11):348-350.
- Breathnach AS, Jenkins DR, Pedler SJ. Stethoscopes as possible vectors of infection by staphylococci. *BMJ*. 1992;305(6868):1573-1574.
- Whittington AM, Whitlow G, Hewson D, Thomas C, Brett SJ. Bacterial contamination of stethoscopes on the intensive care unit. *Anaesthesia*. 2009;64(6):620-624.
- Adams AS, Soumerai SB, Lomas J, Ross-Degnan D. Evidence of self-report bias in assessing adherence to guidelines. *Int J Qual Health Care*. 1999;11(3):187-192.
- Vasudevan R, Shin JH, Chopyk J, et al. Aseptic barriers allow a clean contact for contaminated stethoscope diaphragms. *Mayo Clin Proc Innov Qual Outcomes*. 2020;4(1):21-30.
- Kalra S, Boulee D, Haddock A, Peacock WF. 420 Standard of care for cleaning stethoscopes before patient evaluations. *Ann Emerg Med*. 2017;70(4):S164-S165.
- Muniz J, Sethi RKV, Zaghi J, Zinziel SI, Sandora TJ. Predictors of stethoscope disinfection among pediatric health care providers. *Am J Infect Control*. 2012;40(10):922-925.
- Knecht VR, McGinniss JE, Shankar HM, et al. Molecular analysis of bacterial contamination on stethoscopes in an intensive care unit [published online ahead of print December 18, 2018]. *Infect Control Hosp Epidemiol*. <https://doi.org/10.1017/ice.2018.319>.
- Pidot SJ, Gao W, Bultjens AH, et al. Increasing tolerance of hospital *Enterococcus faecium* to handwash alcohols. *Sci Transl Med*. 2018;10(452). eaar6115.
- O'Flaherty N, Fenelon L. The stethoscope and healthcare-associated infection: a snake in the grass or innocent bystander? *J Hosp Infect*. 2015;91(1):1-7.
- Zaghi J, Zhou J, Graham DA, Potter-Bynoe G, Sandora TJ. Improving stethoscope disinfection at a children's hospital. *Infect Control Hosp Epidemiol*. 2013;34(11):1189-1193.
- Holleck JL, Merchant N, Lin S, Gupta S. Can education influence stethoscope hygiene? *Am J Infect Control*. 2017;45(7):811-812.
- Siegel J, Rhinehart E, Jackson M, Chiarello L. Health Care Infection Control Practices Advisory Committee. 2007 Guideline for isolation precautions: preventing transmission of infectious agents in healthcare settings. *Am J Infect Control*. 2007;35(10 suppl 2):S65-S164.
- Marshall C, Richards M, McBryde E. Do active surveillance and contact precautions reduce MRSA acquisition? A prospective interrupted time series. *PLoS One*. 2013;8(3):e58112.
- Khasawneh F, Mehmood M, Abugrara H, Stewart J. Comparing the auscultatory accuracy of health care professionals using three different brands of stethoscopes on a simulator. *Med Devices Evid Res*. 2014;7:273-281.
- Marinella MA, Pierson C, Chenoweth C. The stethoscope. A potential source of nosocomial infection? *Arch Intern Med*. 1997;157(7):786-790.
- Jenkins IH, Monash B, Wu J, Amin A. The third hand: low rates of stethoscope hygiene on general medical services. *J Hosp Med*. 2015;10(7):457-458.
- Boulee D, Kalra S, Haddock A, Johnson TD, Peacock WF. Contemporary stethoscope cleaning practices: what we haven't learned in 150 years. *Am J Infect Control*. 2019;47(3):238-242.
- Zachary KC, Bayne PS, Morrison VJ, Ford DS, Silver LC, Hooper DC. Contamination of gowns, gloves, and stethoscopes with vancomycin-resistant enterococci. *Infect Control Hosp Epidemiol*. 2001;22(9):560-564.
- Parmar RC, Valvi CC, Sira P, Kamat JR. A prospective, randomised, double-blind study of comparative efficacy of immediate versus daily cleaning of stethoscope using 66% ethyl alcohol. *Indian J Med Sci*. 2004;58(10):423-430.
- Kalra S, Shewale JB, Peacock WF. Are stethoscopes and infection control enemies? *Ann Emerg Med*. 2020;76(4S):S99.
- Schmidt MG, Tuuri RE, Dharsee A, et al. Antimicrobial copper alloys decreased bacteria on stethoscope surfaces. *Am J Infect Control*. 2017;45(6):642-647.
- Messina G, Burgassi S, Messina D, Montagnani V, Cevenini G. A new UV-LED device for automatic disinfection of stethoscope membranes. *Am J Infect Control*. 2015;43(10):e61-e66.
- Wood MW, Lund RC, Stevenson KB. Bacterial contamination of stethoscopes with antimicrobial diaphragm covers. *Am J Infect Control*. 2007;35(4):263-266.