

UC Santa Barbara

UC Santa Barbara Previously Published Works

Title

Precise Electrochemical Sizing of Individual Electro-Inactive Particles.

Permalink

<https://escholarship.org/uc/item/5dw0z0cw>

Authors

Chung, Julia

Plaxco, Kevin

Sepunaru, Lior

Publication Date

2023-08-04

DOI

10.3791/65116

Peer reviewed



Precise Electrochemical Sizing of Individual Electro-Inactive Particles

Julia Chung¹, Kevin W. Plaxco^{1,2}, Lior Sepunaru²

¹Interdepartmental Program in Biomedical Science and Engineering, University of California at Santa Barbara

²Department of Chemistry and Biochemistry, University of California at Santa Barbara

Abstract

Nanoimpact electrochemistry enables the time-resolved *in situ* characterization (e.g., size, catalytic activity) of single nanomaterial units, providing a means of elucidating heterogeneities that would be masked in ensemble studies. To implement this technique with redox inactive particles, a solution-phase redox reaction is used to produce a steady-state background current on a disk ultramicroelectrode. When a particle adsorbs onto the electrode, it produces a stepwise reduction in the exposed electrode area, which produces, in turn, a stepwise decrease in the current commensurate with the size of the adsorbing species. Historically, however, nanoimpact electrochemistry has suffered from “edge effects,” in which the radial diffusion layer formed at the circumference of the ultramicroelectrodes renders the step size dependent not only on the size of the particle but also on where it lands on the electrode. The introduction of electrocatalytic current generation, however, mitigates the heterogeneity caused by edge effects, thus improving the measurement precision. In this approach, termed “electrocatalytic interruption,” a substrate that regenerates the redox probe at the diffusion layer is introduced. This shifts the rate-limiting step of the current generation from diffusion to the homogeneous reaction rate constant, thus reducing flux heterogeneity and increasing the precision of particle sizing by an order of magnitude. The protocol described here explains the set-up and data collection employed in nanoimpact experiments implementing this effect for improved precision in the sizing of redox in-active materials.

Introduction

Nanoimpact electrochemistry is an electrochemical technique that enables the time-resolved detection of individual particles *in situ* in a sample^{1,2,3,4,5,6,7}. The individual particles that can be characterized by this approach span a wide range of materials^{6,8,9,10,11,12,13} and encompass dimensions from individual atoms to whole cells^{7,8,14,15,16}.

Corresponding Author: Lior Sepunaru, sepunaru@ucsb.edu.

A complete version of this article that includes the video component is available at <http://dx.doi.org/10.3791/65116>.

Disclosures

The authors have nothing to disclose.

To accommodate the detection and characterization of such small materials, the technique utilizes micron- and submicron-scale disk ultramicroelectrodes. The impact of an *electroactive* nanoparticle on such an electrode produces an easily quantifiable current change as the nanoparticle undergoes a redox reaction. To expand this to the detection of electro-*inactive* materials, a background electrochemical reaction is used to produce a steady-state current that is reduced in a step-wise fashion as the adsorption of the nanoparticles changes the surface area of the electrode¹⁷. In this scheme, ultramicroelectrodes are employed to increase the relative change produced by each nanoimpact. The radial diffusion layer that such microelectrodes produce, however, reduces the measurement precision due to “edge effects”¹⁸. These occur because the flux of the redox species to the electrode is greater at the edges of the electrode than at its center¹⁹. Thus, when a single nanoparticle lands at the edge of the electrode surface, the resulting current event is larger than that seen for an identical particle landing at the center of the electrode¹⁹, and this effect is more significant for ultramicroelectrodes due to their small area-to-circumference ratio. These edge effects detract significantly from the precision of nanoimpact electrochemistry; due to their presence, the estimated particle size distributions produced by nanoimpact sizing are 20 times wider than those obtained using “gold standard” microscopy techniques²⁰. This reduced precision detracts from the use of nanoimpact electrochemistry as an analytical technique for evaluating the heterogeneity of redox inactive materials at the nanoscale^{4,17,19,21,22,23,24,25,26}.

We have recently introduced a method (Figure 1) that mitigates edge effects in nanoimpact approaches²⁰. In this method, the introduction of a substrate regenerates the redox species near the ultramicroelectrode surface. This shifts the rate-limiting step in current generation from diffusion to the rate of the homogeneous chemical reaction of the redox species in solution^{27,28}, thus reducing the extent to which the radial diffusion field contributes to heterogeneous currents. Specifically, the oxidation of 2,2,6,6-tetramethylpiperidine 1-oxyl (TEMPO) provides the background redox reaction at the ultramicroelectrode²⁹. The addition of maltose to this regenerates the reduced form of TEMPO^{30,31}. This regeneration is rapid³², and it compresses the diffusion layer and reduces the current heterogeneity associated with spatial landing²⁰. As a result, the “electrocatalytic interruption” approach improves the precision of nanoimpact particle sizing by an order of magnitude.

Protocol

1. Establishing a low-noise system

NOTE: The relevant experiments require a potentiostat capable of achieving the highly time-resolved measurement of low currents. To achieve this, employ a research-grade commercial potentiostat capable of a 1 μ s time resolution that can quantify currents at the femtoampere level. To further reduce electronic interference from the environment, conduct experiments within two nesting Faraday cages. Ensure that the setup is capable of a root-mean-square deviation of less than 100 fA for a chronoamperometry experiment sampled at 10 Hz in 0.1 M potassium chloride.

1. Obtain and set up the equipment, including the potentiostat and Faraday cages.

NOTE: Faraday cages may be obtained commercially or custom-fabricated using conductive metals (e.g., copper or aluminum). Custom-fabricated aluminum Faraday cages were used for the study described here (see Table of Materials).

2. Experimental preparation

1. Use commercially available 2 μm diameter carboxylatemoified polystyrene beads (see Table of Materials).

NOTE: While this system can be generalized to other electro-inactive species^{23,33}, it is critical to remember that the impacts rely on electrophoretic migration in addition to Brownian motion. Thus, apply a potential attractive to the species of interest, and maintain low salt concentrations¹⁷.

2. Prepare the following solutions, which can be stored at room temperature for at least 1 month.
 1. Prepare a 50 mM carbonate solution, and titrate to pH 12.0 using 1 M NaOH. Monitor the pH weekly.
 2. Prepare a 1 M sodium perchlorate solution.
3. Prepare the following solutions fresh each day, discarding them at the end of the day.
 1. Prepare a 10 mM TEMPO in 50 mM carbonate solution, pH 12.0.
 2. Prepare a 500 mM maltose stock in 50 mM carbonate solution, pH 12.0.
4. Select the working electrode. For consistent results, select an ultramicroelectrode (see Table of Materials) such that the radius of the species to be characterized is no less than 10%–15% of the electrode radius^{17,21,23,33,34}.

NOTE: This ratio can be minimized after determining the magnitude of the impact-associated current steps for the optimal detection of a particular species of interest. The electrode material selected must catalyze the background redox reaction.

5. Prepare two electrochemical cells of 5 mL each.
 1. Prepare a control cell containing 1 mM TEMPO and 5 mM sodium perchlorate (see Table of Materials) in carbonate buffer at pH 12.0.
 2. Prepare a test cell containing a solution of 1 mM TEMPO, 5 mM sodium perchlorate, and 120 mM maltose in carbonate buffer at pH 12.0.

NOTE: The ratio of the redox mediator to the substrate (here, TEMPO to maltose) can be varied to explore the effects of the reaction rate²⁰. This value provides insight into the homogeneous chemical reaction.

3. After preparing these cells, set them aside for later electrochemical measurements.

3. Electrode polishing

1. Prior to each experimental run, polish the electrode sequentially for 2 min each with a 1 μm , 0.3 μm , and 0.5 μm alumina slurry (see Table of Materials) on polishing pads.
2. Move the electrode in a “figure 8” pattern to ensure an even polish^{35,36}. Liberally rinse with deionized water, and dry with a laboratory wipe.

NOTE: Do not sonicate the ultramicroelectrodes, as this may damage them.

4. Electrochemical measurements

NOTE: See Figure 2 for the results.

1. Utilize a three-electrode setup for the electrochemical measurements. For the experiments described here, employ an 11 μm carbon-fiber ultramicroelectrode, a platinum wire counter electrode, and a saturated calomel reference electrode (SCE) (see Table of Materials).

NOTE: Electrochemical potential windows for the experiments are noted below; for reference, TEMPO has a formal potential of 0.49 V versus SCE, and maltose is not electroactive in the potential window used in these experiments. Any leaking from the reference electrode may affect the total salt concentration³⁷, thus reducing the electrophoretic driving of the particles to the ultramicroelectrode and reducing the counting efficiency¹⁷. If the experiments yield a low impact frequency, consider switching to a leakless reference electrode^{38,39}.

2. Set the control cell in the Faraday cages, and connect the electrodes to the appropriate cables. Collect the first set of electrochemical measurements for each cell. This will consist of a cyclic voltammetry experiment and a chronoamperometry experiment, as detailed below.
 1. Collect the cyclic voltammetry data using a potential window from 0.2 V to 0.8 V versus SCE at scan rates of 10 $\text{mV}\cdot\text{s}^{-1}$, 20 $\text{mV}\cdot\text{s}^{-1}$, 30 $\text{mV}\cdot\text{s}^{-1}$, 40 $\text{mV}\cdot\text{s}^{-1}$, and 50 $\text{mV}\cdot\text{s}^{-1}$.
 2. Collect the chronoamperometry data by applying 0.8 V versus SCE for 10 min, and record at a 10 Hz sampling rate.

NOTE: A 10 min sampling period is recommended for chronoamperometry experiments to obtain 10–15 individual impacts at later steps. No impacts are expected at this juncture.

3. Next, spike a dilute solution of polystyrene beads to a final concentration of 0.66 pM ¹⁷ into each of the electrochemical cells. After the addition of the polystyrene beads, collect the second set of electrochemical measurements for each cell.

NOTE: The impact frequency will be a function of this concentration and requires optimization to collect sufficient data for statistical analysis without saturating the chronoamperogram with overlapping impacts^{40,41,42,43}.

1. Collect chronoamperometry data by applying 0.8 V versus SCE for 10 min, and record at a 10 Hz sampling rate.
2. Repeat the chronoamperometric measurements until sufficient data points have been collected for statistical analysis. To detect differences between the multiple sizing methods with a confidence level of 95% and a power of 80%, select a sample size of approximately 200 individual impact events.

5. Scanning electron microscopy (SEM)

NOTE: Use scanning electron microscopy as a “gold standard” technique to confirm the nanoparticle sizes and sample heterogeneity^{19,44}.

1. Sample preparation
 1. To prepare a sample for imaging, dilute a carboxyl latex bead suspension (see Table of Materials) 1:20 in water. Drop-cast 10 μL onto a glass slide, dry under a nitrogen stream, and sputter-coat the sample with a conductive layer of gold-palladium under argon.
2. Imaging
 1. Using an accelerating beam voltage of 5 kV and a current of 0.4 nA, collect images as appropriate for statistical analysis. Use ImageJ^{45,46} or an equivalent image analysis software to determine the particle sizes.

6. Electrochemical data analysis

1. Record the electrochemical data using the potentiostat’s software, and analyze these results using a written script²⁰ that can extract the current magnitudes from the detected changes in the steady-state current (current steps) resulting from nanoimpact events²⁰.

NOTE: This script is included as part of the supplemental information in our previously published report²⁰.

2. Convert the amplitudes of the current steps to bead radii using the following equation:

$$r_b = \sqrt{\frac{\Delta I_{ss}}{I_{ss}} \frac{1}{f_{(MMT, Geom)}}} r_{el}^2$$

NOTE: Here, r_b is the bead radius, r_{el} is the electrode radius, $\Delta I_{ss}/I_{ss}$ is the ratio between the change in the current produced by a particle’s adsorption and the initial steady-state current observed prior to the adsorption of that particle, and $f_{(MT, Geom)} = 0.067$ is an empirical scaling factor that depends on both geometric and mass transport considerations^{20,25}.

3. Plot the frequency of detecting a given bead radius versus the radius (Figure 3) to quantify the distribution metrics.

7. Modeling

NOTE: If desired, the mechanism by which electrocatalytic interruption works can be validated by confirming the shift from the diffusion-limited current generation to the reaction rate-limited current generation. To describe and visualize, use two different numerical simulation programs: a voltammogram fitting software, such as DigiSim, to determine the homogeneous rate constant, and a multiphysics modeling platform, such as COMSOL Multiphysics, to visualize the local changes to the diffusion profile at the ultramicroelectrode surface (see Table of Materials).

1. Voltammogram fitting

NOTE: Use the voltammogram fitting software to determine the homogeneous rate constant (Figure 4).

1. Collect cyclic voltammograms in a solution containing 1 mM TEMPO (only) and 1 mM TEMPO plus 120 mM maltose. For each condition, collect data at various scan rates, and use this data for numerical fittings of these experimental datasets.
 1. Fit the voltammograms collected from the TEMPO-only experiment using an E mechanism, which describes a reaction process driven solely by the electrode^{47,48}. This will yield the electrode parameters.
 2. Using the electrode parameters obtained from step 7.1.1.1, fit the resulting voltammograms from the 1 mM TEMPO plus 120 maltose solution to an EC' mechanism^{47,48}, which describes an electrode process that is followed by a homogeneous chemical reaction that regenerates the redox mediator. This will yield the homogeneous rate constant.

2. Multiphysics modeling

1. Use a multiphysics modeling platform to visualize the changes in the diffusion profiles at the ultramicroelectrode surface for both the control and electrocatalytic interruption systems^{20,49,50,51,52} (Figure 5). Use the electrode parameters and homogeneous rate constant obtained from the voltammogram fitting as initial conditions. A broad overview of the workflow, which can be adapted to different software, is provided below.
2. Input the global parameters. These consist of fixed values such as (but not limited to) the concentration values, diffusion coefficients, electrode radius, and temperature.
3. Build the simulation space. This is a set of geometries that include the electrode, the insulating sheath, the surrounding solution space representing the region of interest, and an infinite element domain representing the bulk surroundings.

4. Introduce physics packages to define the simulation.
 1. Associate the electrode space with an electroanalysis study. Define the initial values and electrode reaction of interest here.
 2. Associate the surrounding solution space with a chemistry study. Define the homogeneous chemical reaction that follows the electrode reaction here.
 3. Introduce a mesh over the entire simulation space. This defines how the geometry is divided to solve the model. To achieve high-quality results, use a finer mesh near the electrode.
5. To observe changes as a result of the homogeneous rate constant, vary the value of this parameter using a parametric study to solve the model.
6. To observe changes as a function of time, vary the value of this parameter using a time-dependent study to solve the model.

Representative Results

Electrocatalytic interruption mitigates edge effects by shifting the primary current generation mechanism from diffusion-limited (i.e., limited by the transport of a redox probe to the electrode) to kinetically limited (i.e., limited by a rapid, solution-phase reaction)²⁰. This method is modular, meaning it allows a mix-and-match approach to choosing the electrode material, redox probe, and substrate, and this renders electrocatalytic interruption amenable to the detection of many nano- and bio-materials^{6,7,8,9,10,11,12,13,14,15,22}. Implementing this technique on a 5.5 μm radius carbon-fiber electrode produced a 10-fold improvement in the precision associated with the electrochemical sizing of a model system (polystyrene beads) in a solution containing TEMPO as a redox probe and maltose as a substrate.

Following this protocol, the data sets required to validate this mechanism and its ability to restore analytical precision when sizing electro-inactive nanoparticles can be obtained. First, the cyclic voltammogram data collected in the absence of polystyrene beads showed a reversible redox event in control experiments involving TEMPO alone. From here, the addition of maltose resulted in an increase in the oxidative peak and a concurrent loss in the reductive peak as the oxidized TEMPO was regenerated by maltose. Second, the chronoamperograms collected under these conditions demonstrated that the steady-state currents at an oxidative potential were higher, consistent with the catalytic amplification observed in the cyclic voltammetry results. This step also suggests that the bulk chemical reaction is maintained by the electrode reaction; thus, any improvements over the control method will last over the measurement duration. However, this alone is insufficient for assessing any improvements to the measurement precision; to do so, chronoamperometry data must be collected in the presence of polystyrene beads.

To assess the sizing precision, chronoamperogram data were collected using 2 μm carboxylated polystyrene beads. Upon their addition, step-wise changes in the chronoamperogram current were observed as individual particles impacted and absorbed

(Figure 2A control, Figure 2B electrocatalytic interruption). Each step-wise change in the steady-state current magnitude was converted to particle radii, and the data were visualized as histograms to compare the distribution from these electrochemical techniques to that of a gold standard technique, such as scanning electron microscopy (Figure 3). This comparison then allowed the characterization of precision metrics associated with each sizing approach.

Modeling was utilized to support these experimental observations. Specifically, fitting the cyclic voltammograms from before yielded parameters that characterized both the electrode reaction and the solution-phase chemical reaction (Figure 4). From the control solution, some sample parameters obtained were $E_r^0 = 0.49$ V, $k_0 = 0.02$ cm \cdot s $^{-1}$, and $\nu = 10$ mV \cdot s $^{-1}$ at $T = 25^\circ$ C. From the test solution, the kinetic parameters that limited current generation could be obtained; specifically, as K_{eq} approaches infinity, $k_{obs} = 2,200$ M $^{-1}\cdot$ s $^{-1}$. The numerical simulations could then use these values as the initial conditions for generating a concentration profile of the redox probe (Figure 5). In the absence of maltose, the resultant diffusion profile was radial, leading to heterogeneous material flux; specifically, more material diffused to the electrode at the edges. The introduction of maltose compressed the diffusion profile, producing, in turn, more homogeneous currents across the electrode surface.

Discussion

Electrocatalytic interruption is easy to implement and reduces the imprecision associated with nanoimpact electrochemistry by an order of magnitude. This enhanced precision directly enables researchers to discriminate between differently sized particles in a mixed solution²⁰. It also enhances the ability to reliably detect redox-inactive particles smaller than the historically reported limit of 15%–20% of the radius of the electrode^{17,21,23,34}.

While electrochemical interruption can accommodate various redox systems for the detection of nanoparticles of various electro-inactive materials, identifying such redox systems has remained a major challenge. The main barrier to implementing electrochemical interruption is identifying a chemical reaction that is rapid enough to significantly reduce the confounding contributions of edge effects. Specifically, while some examples of EC' reactions, wherein an electrode reaction is followed by a chemical reaction that regenerates the electrode reactant, are well characterized in the literature^{29,32,53,54,55}, few are sufficiently fast to improve the measurement precision. In this study, from those reactions that are sufficiently fast, a TEMPO-maltose system was chosen, and this yielded an observed rate constant of 2,200 M $^{-1}\cdot$ s $^{-1}$. This, in conjunction with multiphysics simulations that demonstrate that faster reaction rates lead to more homogeneous flux at the electrode edge, supports the conclusion that only fast chemical reactions yield several-fold current enhancements at ultramicroelectrodes.

Catalytic interruption does not require data manipulation or modifications to commercially available ultramicroelectrodes. To explain the heterogeneous current magnitudes characteristic of nanoimpact data, Bonezzi and Boika introduced a theoretical model that relates the current step magnitude to particle size²⁵. This analysis, however, heavily relies on averaging the current magnitudes as a function of the collisional frequency. Not only

does this preclude insight into the properties of individual particles, but this technique also remains reliant on the flux of the redox reporter to the electrode and does not remove the problem of edge effects, thus resulting in reduced precision. Deng et al. introduced the first experimental approach to addressing edge effects, utilizing a hemispherical ultramicroelectrode fabricated from mercury⁵¹. Mercury droplet electrodes, however, are toxic, mechanically unstable, and stable over only a limited potential window⁵⁶. Furthermore, fabricating (and maintaining) perfectly hemispherical microelectrodes using other materials remains challenging^{51,52}. More recently, Moazzenzade et al. proposed ring ultramicroelectrodes for nanoimpact characterization⁵². This geometry is promising but requires nanofabrication capabilities. In contrast, catalytic interruption enables nanoimpact experiments with materials universally found in an electrochemistry laboratory.

Acknowledgments

This work was funded by the National Institutes of Health (NIH) grant R35GM142920. The research reported here made use of shared facilities of the UCSB MRSEC (NSF DMR 1720256), a member of the Materials Research Facilities Network (www.mrfn.org). We thank Phoebe Hertler for contributing to the original article this work references. We thank Dr. Claire Chisholm for assisting in the acquisition of the scanning electron microscopy images.

References

1. Heyrovsky M, Jirkovsky J Polarography and voltammetry of ultrasmall colloids: Introduction to a new field. *Langmuir*. 11 (11), 4288–4292 (1995).
2. Kleijn SEF et al. Landing and catalytic characterization of individual nanoparticles on electrode surfaces. *Journal of the American Chemical Society*. 134 (45), 18558–18561 (2012). [PubMed: 23102515]
3. Hill CM, Clayton DA, Pan S Combined optical and electrochemical methods for studying electrochemistry at the single molecule and single particle level: Recent progress and perspectives. *Physical Chemistry Chemical Physics*. 15 (48), 20797–20807 (2013). [PubMed: 24196825]
4. Dick JE, Hilterbrand AT, Boika A, Upton JW, Bard AJ Electrochemical detection of a single cytomegalovirus at an ultramicroelectrode and its antibody anchoring. *Proceedings of the National Academy of Sciences of the United States of America*. 112 (17), 5303–5308 (2015). [PubMed: 25870261]
5. Mirkin MV, Sun T, Yu Y, Zhou M Electrochemistry at one nanoparticle. *Accounts of Chemical Research*. 49 (10), 2328–2335 (2016). [PubMed: 27626289]
6. Sokolov SV, Eloul S, Kätelhön E, Batchelor-McAuley C, Compton RG Electrode-particle impacts: A users guide. *Physical Chemistry Chemical Physics*. 19 (1), 28–43 (2017).
7. Stevenson KJ, Tschulik K A materials driven approach for understanding single entity nano impact electrochemistry. *Current Opinion in Electrochemistry*. 6 (1), 38–45 (2017).
8. Baker LA Perspective and prospectus on single-entity electrochemistry. *Journal of the American Chemical Society*. 140 (46), 15549–15559 (2018). [PubMed: 30388887]
9. Cheng W, Compton RG Electrochemical detection of nanoparticles by ‘nano-impact’ methods. *TrAC Trends in Analytical Chemistry*. 58, 79–89 (2014).
10. Bard AJ, Fan F-RF Electrochemical detection of single molecules. *Accounts of Chemical Research*. 29 (12), 572–578 (1996).
11. Xiao X, Bard AJ Observing single nanoparticle collisions at an ultramicroelectrode by electrocatalytic amplification. *Journal of the American Chemical Society*. 129 (31), 9610–9612 (2007). [PubMed: 17630740]
12. Anderson TJ, Zhang B Single-nanoparticle electrochemistry through immobilization and collision. *Accounts of Chemical Research*. 49 (11), 2625–2631 (2016). [PubMed: 27730817]

13. Goines S, Dick JE Review-Electrochemistry's potential to reach the ultimate sensitivity in measurement science. *Journal of the Electrochemical Society*. 167 (3), 037505 (2020).
14. Kai T, Zhou M, Johnson S, Ahn HS, Bard AJ Direct observation of $C_2O_4^{•-}$ and $CO_2^{•-}$ by oxidation of oxalate within nanogap of scanning electrochemical microscope. *Journal of the American Chemical Society*. 140 (47), 16178–16183 (2018). [PubMed: 30388001]
15. Dick JE Electrochemical detection of single cancer and healthy cell collisions on a microelectrode. *Chemical Communications*. 52 (72), 10906–10909 (2016). [PubMed: 27533129]
16. Sepunaru L, Sokolov SV, Holter J, Young NP, Compton RG Electrochemical red blood cell counting: One at a time. *Angewandte Chemie International Edition*. 55 (33), 9768–9771 (2016). [PubMed: 27355839]
17. Quinn BM, van't Hof PG, Lemay SG Time-resolved electrochemical detection of discrete adsorption events. *Journal of the American Chemical Society*. 126 (27), 8360–8361 (2004). [PubMed: 15237976]
18. Oldham KB Edge effects in semiinfinite diffusion. *Journal of Electroanalytical Chemistry and Interfacial Electrochemistry*. 122, 1–17 (1981).
19. Fosdick SE, Anderson MJ, Nettleton EG, Crooks RM Correlated electrochemical and optical tracking of discrete collision events. *Journal of the American Chemical Society*. 135 (16), 5994–5997 (2013). [PubMed: 23590646]
20. Chung J, Hertler P, Plaxco KW, Sepunaru L Catalytic interruption mitigates edge effects in the characterization of heterogeneous, insulating nanoparticles. *Journal of the American Chemical Society*. 143 (45), 18888–18898 (2021). [PubMed: 34735140]
21. Boika A, Thorgaard SN, Bard AJ Monitoring the electrophoretic migration and adsorption of single insulating nanoparticles at ultramicroelectrodes. *The Journal of Physical Chemistry B*. 117 (16), 4371–4380 (2013). [PubMed: 23092206]
22. Kim B-K, Boika A, Kim J, Dick JE, Bard AJ Characterizing emulsions by observation of single droplet collisions-Attoliter electrochemical reactors. *Journal of the American Chemical Society*. 136 (13), 4849–4852 (2014). [PubMed: 24641496]
23. Dick JE, Renault C, Bard AJ Observation of single-protein and DNA macromolecule collisions on ultramicroelectrodes. *Journal of the American Chemical Society*. 137 (26), 8376–8379 (2015). [PubMed: 26108405]
24. Lee JY, Kim B-K, Kang M, Park JH Label-free detection of single living bacteria via electrochemical collision event. *Scientific Reports*. 6 (1), 30022 (2016). [PubMed: 27435527]
25. Bonezzi J, Boika A Deciphering the magnitude of current steps in electrochemical blocking collision experiments and its implications. *Electrochimica Acta*. 236, 252–259 (2017).
26. Ellison J, Batchelor-McAuley C, Tschulik K, Compton RG The use of cylindrical micro-wire electrodes for nano-impact experiments; Facilitating the sub-picomolar detection of single nanoparticles. *Sensors and Actuators B: Chemical*. 200, 47–52 (2014).
27. Denuault G, Fleischmann M, Pletcher D, Tutty OR Development of the theory for the interpretation of steady state limiting currents at a microelectrode: EC' processes: First and second order reactions. *Journal of Electroanalytical Chemistry and Interfacial Electrochemistry*. 280 (2), 243–254 (1990).
28. Francke R, Little RD Redox catalysis in organic electrosynthesis: Basic principles and recent developments. *Chemical Society Reviews*. 43 (8), 2492–2521 (2014). [PubMed: 24500279]
29. Nutting JE, Rafiee M, Stahl SS Tetramethylpiperidine N-Oxyl (TEMPO), phthalimide N-oxyl (PINO), and related N-Oxyl species: Electrochemical properties and their use in electrocatalytic reactions. *Chemical Reviews*. 118 (9), 4834 (2018). [PubMed: 29707945]
30. Pierre G et al. TEMPO-mediated oxidation of polysaccharides: An ongoing story. *Carbohydrate Polymers*. 165, 71–85 (2017). [PubMed: 28363578]
31. Liaigre D, Breton T, Belgsir EM Kinetic and selectivity control of TEMPO electro-mediated oxidation of alcohols. *Electrochemistry Communications*. 7 (3), 312–316 (2005).
32. Rafiee M, Karimi B, Alizadeh S Mechanistic study of the electrocatalytic oxidation of alcohols by TEMPO and NHPI. *ChemElectroChem*. 1 (2), 455–462 (2014).
33. Deng Z, Renault C Detection of individual insulating entities by electrochemical blocking. *Current Opinion in Electrochemistry*. 25, 100619 (2021).

34. Laborda E, Molina A, Batchelor-McAuley C, Compton RG Individual detection and characterization of non-electrocatalytic, redox-inactive particles in solution by using electrochemistry. *ChemElectroChem*. 5 (3), 410–417 (2018).
35. Elgrishi N et al. A practical beginner's guide to cyclic voltammetry. *Journal of Chemical Education*. 95 (2), 197–206 (2018).
36. Cardwell TJ, Mocak J, Santos JH, Bond AM Preparation of microelectrodes: comparison of polishing procedures by statistical analysis of voltammetric data. *Analyst*. 121 (3), 357–362 (1996).
37. Lämmel C, Heubner C, Liebmann T, Schneider M Critical impact of chloride containing reference electrodes on electrochemical measurements. *Electroanalysis*. 29 (12), 2752–2756 (2017).
38. Walker NL, Dick JE Leakless, bipolar reference electrodes: Fabrication, performance, and miniaturization. *Analytical Chemistry*. 93 (29), 10065–10074 (2021). [PubMed: 34263595]
39. Troutd BK, Rousseau CR, Dong XIN, Anderson EL, Bühlmann P Recent progress in the development of improved reference electrodes for electrochemistry. *Analytical Sciences*. 38 (1), 71–83 (2022). [PubMed: 35287207]
40. Stuart EJE, Zhou Y-G, Rees NV, Compton RG Particle-impact nanoelectrochemistry: A Fickian model for nanoparticle transport. *RSC Advances*. 2 (33), 12702–12705 (2012).
41. Boika A, Bard AJ Time of first arrival in electrochemical collision experiments as a measure of ultralow concentrations of analytes in solution. *Analytical Chemistry*. 87 (8), 4341–4346 (2015). [PubMed: 25803279]
42. Robinson DA et al. Collision dynamics during the electrooxidation of individual silver nanoparticles. *Journal of the American Chemical Society*. 139 (46), 16923–16931 (2017). [PubMed: 29083174]
43. Lemay SG, Moazzenzade T Single-entity electrochemistry for digital biosensing at ultralow concentrations. *Analytical Chemistry*. 93 (26), 9023–9031 (2021). [PubMed: 34167291]
44. Vernon-Parry KD Scanning electron microscopy: An introduction. *III-Vs Review*. 13 (4), 40–44 (2000).
45. Abramoff MD, Magalhães PJ, Ram SJ Image processing with ImageJ. *Biophotonics International*. 11 (7), 36–42 (2004).
46. Collins TJ ImageJ for microscopy. *BioTechniques*. 43 (1S), S25–S30 (2007).
47. Bard AJ, Faulkner LR *Electrochemical Methods: Fundamentals and Applications*. Wiley. New York, NY (2001).
48. Compton RG, Banks CE *Understanding Voltammetry (Third Edition)*. World Scientific. Singapore (2018).
49. Cutress IJ, Dickinson EJJ, Compton RG Analysis of commercial general engineering finite element software in electrochemical simulations. *Journal of Electroanalytical Chemistry*. 638 (1), 76–83 (2010).
50. Dickinson EJJ, Ekström H, Fontes E COMSOL Multiphysics®: Finite element software for electrochemical analysis. A mini-review. *Electrochemistry Communications*. 40, 71–74 (2014).
51. Deng Z, Elattar R, Maroun F, Renault C In situ measurement of the size distribution and concentration of insulating particles by electrochemical collision on hemispherical ultramicroelectrodes. *Analytical Chemistry*. 90 (21), 12923–12929 (2018). [PubMed: 30284818]
52. Moazzenzade T, Walstra T, Yang X, Huskens J, Lemay SG Ring ultramicroelectrodes for current-blockade particle-impact electrochemistry. *Analytical Chemistry*. 94 (28), 10168–101747 (2022). [PubMed: 35792954]
53. Nekrassova O et al. The oxidation of cysteine by aqueous ferricyanide: A kinetic study using boron doped diamond electrode voltammetry. *Electroanalysis*. 14 (21), 1464–1469 (2002).
54. Kuss S, Compton RG Electrocatalytic detection of ascorbic acid using N,N,N',N'-tetramethyl-paraphenylene-diamine (TMPD) mediated oxidation at unmodified gold electrodes; Reaction mechanism and analytical application. *Electrochimica Acta*. 242, 19–24 (2017).
55. Shayani-Jam H, Nematollahi D Electrochemically mediated oxidation of glutathione and N-acetylcysteine with 4,4'-biphenol. *Electrochimica Acta*. 56 (25), 9311–9316 (2011).

56. Vyskočil V, Barek J Mercury electrodes-Possibilities and limitations in environmental electroanalysis. *Critical Reviews in Analytical Chemistry*. 39 (3), 173–188, (2009).

Author Manuscript

Author Manuscript

Author Manuscript

Author Manuscript

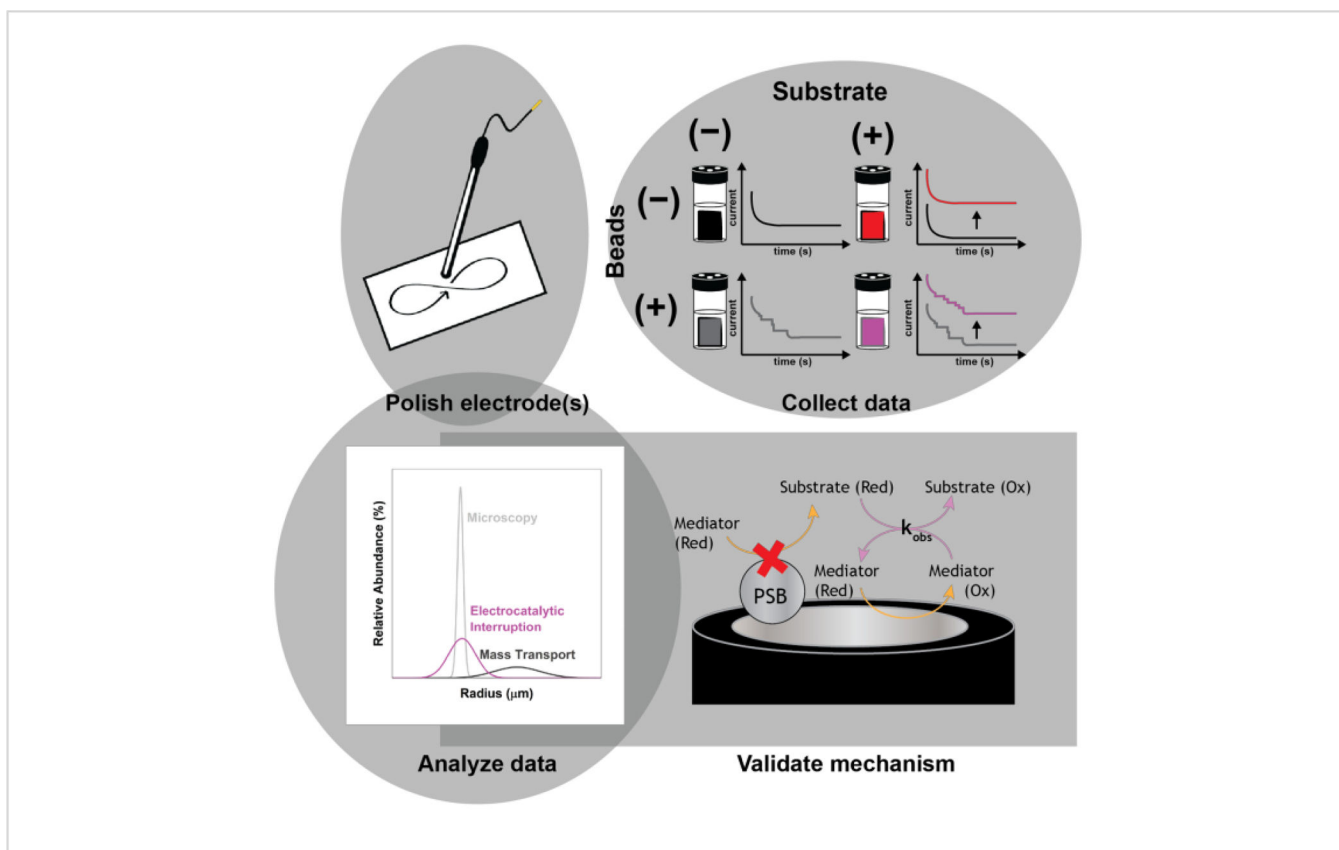


Figure 1: Schematic of the experimental protocol.

Polish the electrodes prior to each experimental run. Collect a baseline set of electrochemical measurements (cyclic voltammetry and chronoamperometry) in the absence of beads with and without implementing electrocatalytic interruption to observe the current enhancement with the addition of the substrate. Spike in the beads, and collect a second set of electrochemical measurements for the size determination of the impacting nanoparticles. Validate the mechanism of action using numerical simulations.

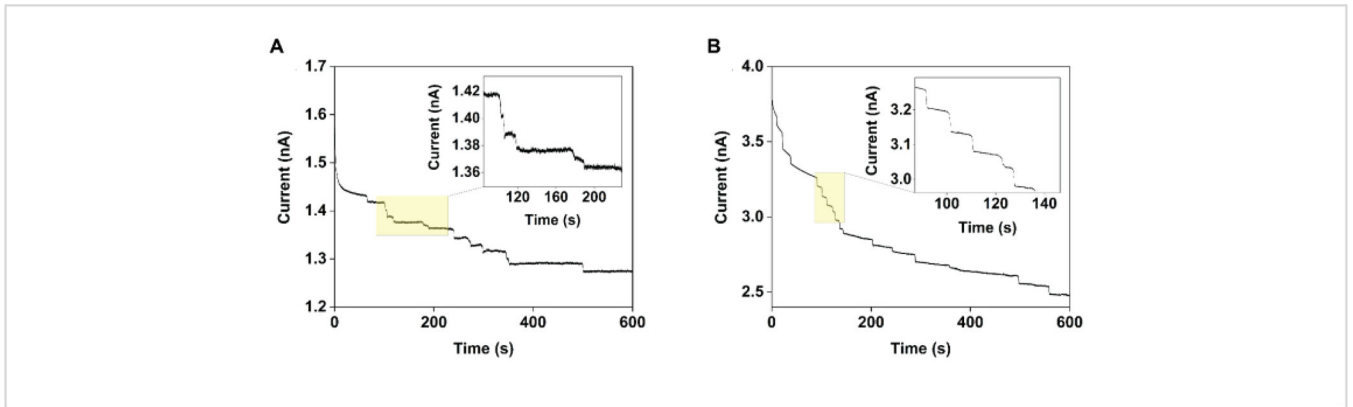


Figure 2: Chronoamperograms collected using an 11 μm diameter carbon-fiber ultramicroelectrode demonstrating the improvement in measurement precision achieved using electrocatalytic interruption.

Specifically, when measuring the current versus time in a solution of 1 mM TEMPO in the (A) absence (control) and (B) presence of 120 mM maltose (electrocatalytic interruption), the steps observed in the latter case were more homogeneous. Reprinted with permission from Chung et al.²⁰.

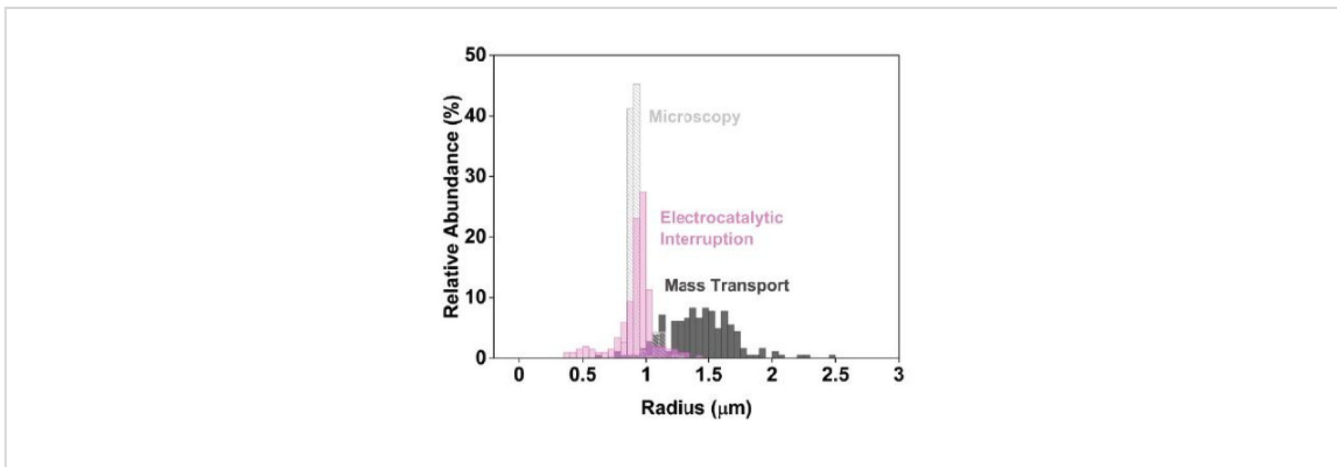


Figure 3: Precise electrochemical sizing data when using electrocatalytic interruption compared to the conventional, diffusion-limited electrochemical approach.

To represent this data, prepare histograms comparing the size distributions determined using scanning electron microscopy (light grey) and electrochemistry (electrocatalytic interruption, pink; control, dark grey). Conventional nanoimpact studies, in which the current is limited by the mass transport of the mediator, produce artificially broad estimated size distributions (dark grey). In contrast, implementing electrocatalytic interruption leads to narrower, more precise size estimations (pink). Reprinted with permission from Chung et al.²⁰.

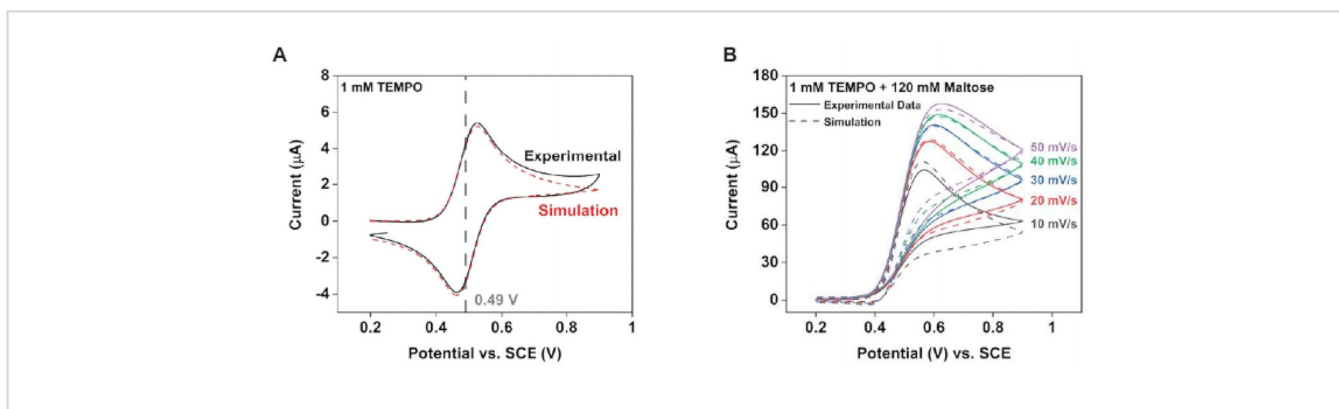


Figure 4: Modeling the electrode kinetics to characterize the new reaction scheme.

Using cyclic voltammogram fitting software, extract the electrode reaction parameters from the experimental data. **(A)** Data with 1 mM TEMPO. **(B)** Data with 1 mM TEMPO plus 120 mM maltose. Reprinted with permission from Chung et al.²⁰.

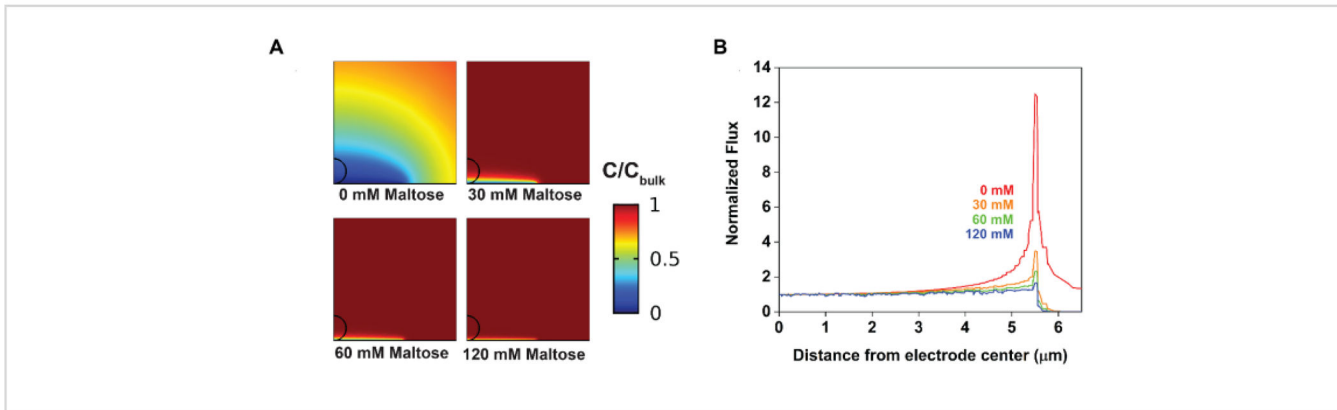


Figure 5: Changes in material flux at the electrode surface upon introducing electrocatalytic interruption visualized by numerical simulations.

(A) The addition of maltose compresses the diffusion layer in a concentration-dependent manner. (B) The addition of maltose depresses the heterogeneous flux at the electrode edges. Reprinted with permission from Chung et al.²⁰.

Materials

Name	Company	Catalog Number	Comments
0.05 μm microalumina polish	Buehler	4010075	
0.3 μm microalumina polish	Buehler	4010077	
1 μm microalumina polish	Buehler	4010079	
20 mL scintillation vials	Fisher Sci	03-339-26C	
Analytical balance	Ohaus		
Apreo C LoVac FEG SEM	Thermo Fisher		
Carbon fiber microelectrode	ALS	002007	Working electrode; purchased from CH Instruments
Carboxyl Latex Beads, 4% w/v, 2 μm	ThermoFisher Scientific	C37278	
COMSOL Multiphysics	COMSOL Multiphysics	v6.0	
D-(+)-Maltose monohydrate	Sigma Aldrich	M5885	
DigiSim	Bioanalytical Systems, Inc.	v3.03b	Discontinued; comparable software is available commercially through the same vendor
EC-Lab	BioLogic	v11.27	
Faraday cages			Custom; analogous equipment can be commercially purchased or fabricated of conductive sheet metals (e.g., copper or aluminum)
Hummer Sputter Coater	Anatech USA		
OriginPro	OriginLab	v2022b	
P1000 micropipette	Fisher Scientific		
P2 micropipette	Fisher Scientific		
P20 micropipette	Fisher Scientific		
P200 micropipette	Fisher Scientific		
Platinum Wire Electrode	CH Instruments	CHI115	Counter electrode
Potassium chloride	Sigma Aldrich	P3911	
PSA-backed MicroCloth	Buehler	407218	
Saturated Calomel Electrode	CH Instruments	CHI150	Reference electrode
Sodium carbonate	Fisher Chemical	S263	
Sodium hydroxide	Sigma Aldrich	S8045	
Sodium perchlorate	EM Science	SX0692	
SP-300	BioLogic		
TEMPO	Oakwood Chemical	013714	
Ultra Low Current module	BioLogic		