

## UC Davis

### UC Davis Previously Published Works

**Title**

Refractometer assessment of colostral and serum IgG and milk total solids concentrations in dairy cattle

**Permalink**

<https://escholarship.org/uc/item/6kn9c04j>

**Journal**

BMC Veterinary Research, 10(1)

**ISSN**

1746-6148

**Authors**

Chigerwe, Munashe  
Hagey, Jill V

**Publication Date**

2014-12-01

**DOI**

10.1186/s12917-014-0178-7

Peer reviewed

RESEARCH ARTICLE

Open Access

# Refractometer assessment of colostrum and serum IgG and milk total solids concentrations in dairy cattle

Munashe Chigerwe\* and Jill V Hagey

## Abstract

**Background:** Estimation of the quantity of colostrum IgG or serum IgG absorbed following ingestion of colostrum by calves is essential for monitoring the effectiveness of colostrum feeding practices on dairy farms. Milk total solids concentrations determination is a critical part of quality assessment of nonsaleable whole milk prior to feeding to calves. To date, on-farm methods to assess colostrum IgG, serum IgG or milk total solids concentrations have been performed separately with various instruments. The objective of this study was to evaluate the diagnostic performance of a single electronic, hand-held refractometer for assessing colostrum and serum IgG concentrations and milk total solids in dairy cattle. Colostrum IgG, serum IgG and milk total solids concentrations were determined by the refractometer. Corresponding analysis of colostrum and serum IgG concentrations were determined by radial immunodiffusion (RID) while milk total solids were determined by spectrophotometry. Sensitivity and specificity of the refractometer for colostrum and serum samples were calculated as determined by RID. Sensitivity and specificity of the refractometer for milk samples was calculated as determined by spectrophotometry.

**Results:** The sensitivity of the refractometer was 1 for colostrum IgG, serum IgG and milk total solids determinations. Specificity of the refractometer was 0.66, 0.24 and 0 for colostrum IgG, serum IgG and milk total solids determinations, respectively. The refractometer underestimated colostrum IgG, serum IgG and milk total solids concentrations compared to the concentrations determined by RID or spectrophotometry.

**Conclusions:** The refractometer was an acceptable, rapid, convenient on-farm method for determining colostrum IgG and milk total solids. The refractometer was not an acceptable method for determination of serum IgG concentrations as it severely underestimated the serum IgG concentrations.

**Keywords:** Colostrum, Milk, Serum, Immunoglobulin, Milk total solids

## Background

Estimation of IgG concentration in colostrum prior to feeding to calves is a useful tool to improve calf health by ensuring adequate transfer of colostrum immunoglobulins. Several on-farm methods for estimating colostrum IgG concentrations have been reported including hydrometers [1,2], weight of first milking colostrum [3], immunoassay [4], and electronic refractometer [5] with variable test sensitivity and levels of practical application. Estimation of the quantity of IgG absorbed following ingestion of colostrum by calves is essential for monitoring

the effectiveness of colostrum feeding practices on dairy farms. Practical methods used for estimating serum IgG following ingestion of colostrum in dairy calves include serum total protein determination by refractometry [6,7], sodium sulfite [8], and turbidimetric methods [9]. Radial immunodiffusion (RID) is considered the reference method for determination of colostrum or serum IgG concentrations and is therefore utilized in diagnostic and laboratory settings [10].

Nonsaleable milk includes postparturient milk collected after the first-milking colostrum for the first few days of a cow's lactation as well as discarded milk from lactating cows undergoing treatment for various disease conditions. Nonsaleable milk can be fed neonatal dairy calves following pasteurization. Milk total solids (sum of percentage fat

\* Correspondence: mchigerwe@ucdavis.edu  
Department of Medicine and Epidemiology, University of California-Davis,  
School of Veterinary Medicine, One Shields Avenue, Davis, CA 95616, USA

and solids non-fat) assessment is critical in the determination of the nutritional value of the nonsaleable milk prior to feeding to calves because the total solids concentrations are variable. In instances where the total solids concentrations are insufficient, additional ingredients such as milk replacer may be added to the milk to achieve target total solids concentrations. Practical methods used to assess whole milk total solids in dairy milk include refractometry [11,12] while spectrophotometry is considered the reference method for evaluating milk total solids [12].

Previous refractometers estimated colostrum IgG or total solids by reporting a Brix value (measure of refractive index), which is then correlated to colostrum IgG or total solid concentrations. Additionally, previous practical methods to estimate colostrum IgG concentration, serum IgG concentrations in calves or total solids in milk were performed separately with different instruments. A more practical approach would be utilization of a single on-farm instrument that quantitatively reports colostrum IgG, serum IgG and total solids without the need to correlate Brix test results with colostrum or serum IgG concentrations or total solids. To the authors' knowledge, no studies have evaluated the use of a single instrument to quantitatively estimate colostrum or serum IgG concentrations and milk total solids. The purpose of this study was to evaluate the practical diagnostic utility of a single on-farm refractometer capable of estimating colostrum or serum IgG concentrations and milk total solids with test results reported in g/L for colostrum and serum and % total solids for milk.

## Methods

### Samples size calculation and sample collection

Colostrum sample size calculation using previously reported methods [13] were based on reported sensitivity of 0.75 [5] of the electronic refractometer in assessing colostrum quality. Serum sample size determination using previously reported methods [13] was based on the sensitivity of 0.89 [7] of refractometers for assessing passive transfer status in serum of calves. Sample size calculation using standard methods [14] for the required milk samples was based on the previously reported correlation coefficient of 0.93 between the refractometer and spectrophotometry results [12]. In all sample size calculations a power of  $\geq 0.80$  and  $\alpha = 0.05$  was considered. A minimum sample size of 43 colostrum, 39 serum and 54 milk samples were required.

To increase the variability in colostrum or serum IgG concentrations, samples were collected from more than one farm and or from 2 dairy breeds. Fresh, pooled colostrum samples from 3 Jersey dairy farms were collected. Blood samples were collected from 2-day old heifer calves from 2 dairy farms (1 Jersey farm and 1 Holstein farm) followed by serum harvesting by centrifugation

within 2 hours after collection. The colostrum and serum samples were stored at  $-20^{\circ}\text{C}$  until IgG concentration was measured using a hand-held refractometer (Palm Abbe PA203x, Misco, Cleveland, Ohio, USA) and single RID. According to the manufacturer, the refractometer analysis can be performed on non-frozen colostrum or serum as well as colostrum or serum that has been frozen only once. Analysis of colostrum and serum was performed within 8 weeks after collection. Milk samples were collected from a single dairy farm raising both Holsteins and Jersey cows. Total solids were determined by the refractometer and spectrophotometry on non-frozen fresh milk samples. All sample collection and analysis were conducted between June 2013 and October 2103. Permission to collect study samples was granted by the participating dairy farms. The University of California, Davis Animal Care and Use Committee approved the study.

### Sample analysis

Stored colostrum and samples were thawed at room temperature ( $20-24^{\circ}\text{C}$ ) while milk total solids was determined on fresh non-pasteurized milk samples. The scales for milk solids, colostrum or serum IgG on the refractometer were automatically temperature compensated for aqueous sucrose solutions at  $20^{\circ}\text{C}$  between the temperatures of  $10$  and  $40^{\circ}\text{C}$ . An aliquot ( $0.4\text{ ml}$ ) of deionized water was placed on the prism well of the refractometer to obtain a standardized reading as per manufacturer's recommendations. Following removal of the deionized water, the refractometer was set to determine colostrum or serum IgG or milk total solids. An aliquot ( $0.4\text{ ml}$ ) of the samples was placed in the prism well of the refractometer and result displayed within a minute. The refractometer reported colostrum IgG in g/L, serum IgG in g/L and milk total solids in %. Range of measurement for colostrum IgG, serum IgG and milk total solids were  $22-82\text{ g/L}$ ,  $2-25\text{ g/L}$  and  $5-15\%$ , respectively. In order to ensure a wide range of milk total solids, 9 milk samples were diluted 1:2 with Tris buffered saline.

Single RID using a commercial kit (Bovine RID Kit, Triple J Farms, Bellingham, Washington, USA) was performed on the same colostrum and serum samples evaluated by the refractometer. Briefly, RID plates containing specific anti-bovine IgG, agarose gel,  $0.1\text{ M}$  phosphate buffer pH 7.0,  $0.1\%$  sodium azide as a bacteriostatic agent and  $1\text{ }\mu\text{g/ml}$  amphotericin B as an antifungal agent stored in a refrigerator at  $4^{\circ}\text{C}$  were warmed at room temperature ( $20-24^{\circ}\text{C}$ ). An aliquot ( $5\text{ }\mu\text{l}$ ) of the provided reference serum at 3 different concentrations, were pipetted into the first 3 RID wells. An aliquot ( $5\text{ }\mu\text{l}$ ) of serum (diluted 1:2 with phosphate buffered saline) or colostrum samples (diluted 1:4 with phosphate buffered saline) were pipetted into the remaining individual RID

wells. The plates were incubated at room temperature (20-24°C) for 24 hours. The diameters of the zones of precipitation were measured using a digital RID plate reader (RID plate reader, The Binding Site Inc, San Diego, California, USA) after 24 hours. Colostral or serum sample IgG concentrations were determined by comparing the diameter of the zones of precipitation with a standard curve generated by the reference serum. The regression equation generated in this manner ( $R^2 = 0.97-0.99$ ) accurately predicted inoculum IgG concentration. The reference serum was included in all plates to minimize plate-to-plate variations. Minimum detectable IgG concentration was 196 mg/dL using the RID. Milk samples evaluated by the refractometer were analyzed for total solids at a certified dairy analytical laboratory (Sierra Dairy Labs, Tulare, California, USA) by a mid-infrared method [15] using a spectrophotometer (Bently 150, Bently Instruments, Chaska, Minnesota, USA).

#### Data analysis

Normality of data was checked using the Shapiro-Wilk test. When data was normally distributed the mean was reported as the measure of central tendency. For all statistical tests single RID was considered the reference method for determining colostrum and serum IgG concentrations, while spectrophotometry was considered the reference method for determining milk total solids. Descriptive statistics for colostrum or serum IgG concentrations and milk total solids were performed. Samples with colostrum IgG < 22 or > 82 g/L, serum IgG concentrations < 2 or > 25 g/L as determined by the RID were excluded from the study because of the detection limit of the refractometer. Likewise milk samples with total solids < 5 or > 15% as determined by spectrophotometer were excluded from the study.

Diagnostic sensitivity and specificity (95% CI) of the refractometer was calculated based on the test results using 2 × 2 frequency tables [13]. A concentration of < 50 g/L of IgG was considered the cut-off point for indicating colostrum samples with insufficient IgG [1,5]. A cut-off point of < 10 g/L was considered indicative of inadequate colostrum IgG transfer in calf serum [16,17]. A cut-off point of < 12% was considered indicative of insufficient total solids in whole milk [12]. Sensitivity of the refractometer was defined as the probability of a test result indicating an inadequate colostrum (<50 g/L) or serum (<10 g/L) IgG concentrations as determined by means of RID. Specificity of the refractometer was defined as the probability of a test result indicative of an adequate colostrum (≥50 g/L) or serum (≥10 g/L) IgG concentrations as determined by means of RID. Likewise, for milk, the sensitivity of the refractometer was defined as the probability of a test result indicative of inadequate milk total solids (<12%) as determined by

spectrophotometry. Specificity of the refractometer was defined as the probability of a test result indicative of adequate milk total solids (≥12%) as determined by spectrophotometry. As a result of differences in prevalence of colostrum or serum samples with inadequate IgG concentrations or milk samples with inadequate milk total solids, likelihood ratios (prevalence independent) for a positive or negative test were determined instead of predictive values (prevalence dependent) for a positive or negative test. Likelihood ratios were calculated using standard methods as previously described [13].

In order to assess the ability of the refractometer to provide accurate measurements as indicated by how closely the test results matched with RID or spectrophotometry, precision of the refractometer was determined using the Bland-Altman (limits of agreement plots) method [18]. For each sample and the measured analyte (colostrum IgG, serum IgG or milk total solids) the bias was calculated as the concentration determined by RID or spectrophotometer minus the corresponding paired analyte concentration as determined by the refractometer. Mean bias and 95% (mean ± 1.96 SD) limits of agreement were calculated. A positive bias estimation indicated that the refractometer underestimated the concentration of the analyte, whereas a negative bias estimate indicated that the refractometer overestimated the concentration of the analyte compared with concentration of the same analyte as determined by RID or spectrophotometer. Where applicable, data analysis was performed using a commercial statistical software (Prism 6, GraphPad Inc, La Jolla, California, USA). Values of  $P < 0.05$  were considered significant.

#### Results

Sixty-four colostrum, 46 serum and 74 milk samples were collected. Mean ± SD for colostrum and serum IgG concentrations were 61.0 ± 11.1 g/L and 18.5 ± 8.6 g/L, respectively, as determined by RID. Mean ± SD for milk total solids was 10.2 ± 1.7%. Proportion of samples with colostrum IgG < 50 g/L was 17.2% (11/64) and proportion of samples with serum IgG < 10 g/L was 17.4% (8/46) as determined by RID. Proportion of samples with milk total solids < 12% was 87.8% (65/74) as determined by spectrophotometry.

#### Colostrum IgG

Sensitivity and specificity of the refractometer for detecting colostrum samples with < 50 g/L was 1 (95% CI, 1) and 0.66 (95% CI, 0.53-0.79) respectively. Likelihood ratio of a positive test was 2.9 (95% CI, 1). Likelihood ratio for a negative test could not be calculated because there were no false negatives, resulting in a denominator of zero. Mean bias based on the Bland-Altman plots was 9.9 g/L (95% limits of agreement, -3.1-23.0) indicating



that the refractometer underestimated sample colostrum IgG concentrations by 9.9 g/L, on average. The Bland-Altman plot for colostrum IgG determination is represented in Figure 1.

#### Serum IgG concentrations

Sensitivity and specificity of the refractometer for detecting serum samples with IgG < 10 g/L was 1 (95% CI, 1) and 0.24 (95% CI, 0.1-0.38) respectively, as determined by RID. Likelihood ratio of positive test was 1.3 (95% CI, 1). Likelihood ratio for a negative test could not be calculated because there were no false negatives, resulting in a denominator of zero. Mean bias based on the Bland-Altman plots was 11.3 g/L (95% limits of agreement, -0.2-22.8) indicating that the refractometer underestimated sample serum IgG concentrations by 11.3 g/L, on average. The Bland-Altman plot for serum IgG determination is represented in Figure 2.


#### Milk total solids

Sensitivity and specificity for detecting samples with milk total solids < 12% was 1 (95% CI, 1) and 0 (95% CI, 0) respectively, as determined by spectrophotometry. Likelihood ratio for a positive test was 1 (95% CI, 1). Likelihood ratio for a negative test was not determined because there were no true negatives resulting in a denominator of zero. Mean bias based on the Bland-Altman plots was 0.6 (95% limits of agreement, -1.6-2.8) indicating that the refractometer underestimated milk total solids by 0.6% on average. The Bland-Altman plot for milk total solids is represented in Figure 3.

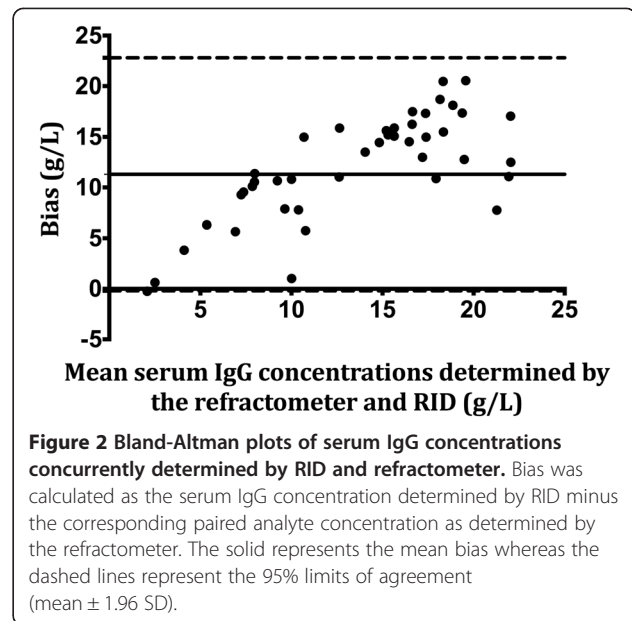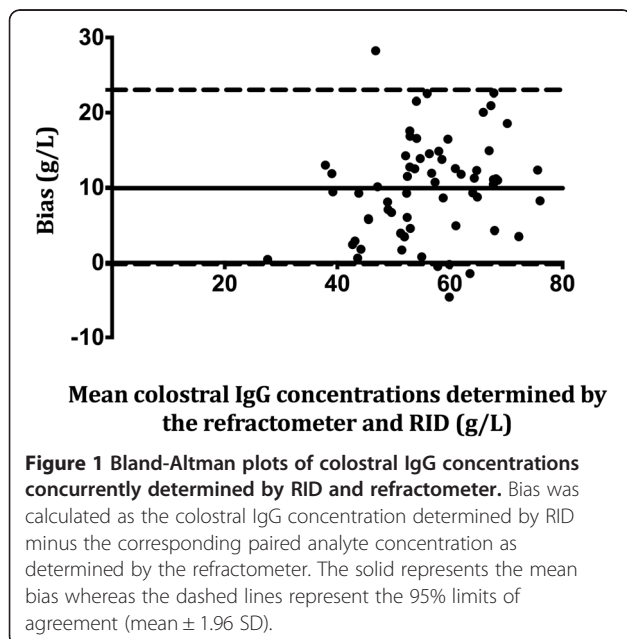

#### Discussion

The main findings from the present study indicated that the refractometer maybe beneficial for the rapid assessment of colostrum IgG and milk total solids but should be used with caution when evaluating serum IgG concentrations in calves. The main advantage of the refractometer over the previous methods for assessing colostrum IgG, serum IgG or milk total solids is the potential convenience of a single instrument that assess all 3 analytes. The refractometer had a sensitivity of 1 for identifying samples with low colostrum IgG, serum IgG or milk total

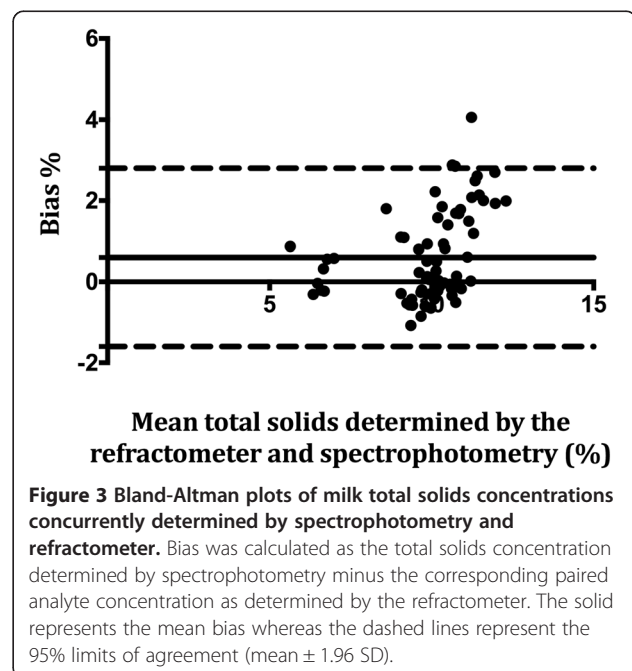

solids concentrations. However, the high sensitivity with a low specificity results in misclassifications of samples with adequate colostrum IgG, serum IgG and milk total solids as inadequate. An effective screening test should have high sensitivity to ensure high predictive value for a negative test and ensure identification of all samples with low colostrum IgG, serum IgG or milk total solids.

The refractometer measures the refractive index. Some refractometers are designed to report the test result as a refractive index [12,19] where as others report the test result as % total solids, as in this study. The refractive index can be used to estimate total solids in cases where the refractometer reports a refractive index. The refractive index varies with the concentration of the compound, temperature of the compound and the wavelength of the light. The refractive index for solutions or transparent liquids with particles sizes between 0.1-0.5  $\mu\text{m}$  in diameter is given by the additive refractive index from each particle [19]. The refractive index of colostrum or milk is considered difficult to measure because of the presence of fat globules, casein micelles and other non-uniform sized globules [20].

Assessment of colostrum IgG concentrations is important to determine the colostrum volume required to be fed to a calf or storage, assuming that 150-200 g total IgG is required for adequate transfer of colostrum immunoglobulins [21]. The refractometer had a higher sensitivity compared to other quantitative methods for assessing colostrum IgG that includes the hydrometer [2,5], refractometer [5] and immunoassay [4]. The advantage of the refractometer (colostrum temperature range for determination, 10-40°C) over the hydrometer (colostrum temperature range for determination, 22-24°C) is that fresh colostrum (mean temperature, 34.6°C) [5] IgG concentration determination does not require cooling. The advantage of the test results of the refractometer reported in this study compared to the previous evaluation of another refractometer [5] is that the reported units are in g/L compared to Brix units. Colostrum IgG reported in g/L are easier to interpret when determining colostrum volume to be fed to the calf compared to Brix units. While another advantage of the refractometer in this study was that it reported a range (22-82 g/L) of colostrum IgG concentration, the immunoassay [4] results were only qualitative (<50 g/L or > 50 g/L). It should be noted that the refractometer underestimated the colostrum IgG concentration by approximately 10 g/L as indicated by the mean bias for the refractometer being 9.9 g/L. The implications of this underestimation of colostrum IgG concentrations is likely to be clinically insignificant as it may only result in increase in volume of colostrum fed to the calf.

Evaluation of passive transfer status in calves is important for monitoring colostrum feeding practices on dairy farms or as part of a treatment management plan

for calves with failure of passive immunity in clinic settings. The sensitivity of 1, of the refractometer for identifying serum samples with IgG concentrations < 10 g/L was higher compared to other common methods used to assess passive transfer status that include serum total protein and sodium sulfite [6,8,22]. The advantage of the refractometer over other practical methods is that it reports serum IgG concentration. However, the mean bias for the refractometer is 11.3 g/L indicating that the refractometer severely underestimated the serum IgG concentrations by 11.3 g/L on average, compared with the RID. Considering that serum IgG concentrations of  $\geq 10$  g/L are considered indicative of adequate transfer of colostrum immunity [16,17], as an example a serum sample result of 5 g/L (indicative failure of passive transfer of colostrum immunity) using this particular digital electronic refractometer may have a true IgG concentration of 16.3 g/L (5 + 11.3), which is indicative of adequate transfer of colostrum immunoglobulins. Thus, practically, using results from this particular refractometer alone for estimating serum IgG concentrations may unnecessarily change colostrum feeding practices on dairy farms or implement inappropriate treatment plan for calves in clinic settings. Therefore, we concluded that the refractometer assessed in study was not an acceptable method for determination of serum IgG concentrations.

Calves fed pasteurized milk had improved weight gain and reduced morbidity and mortality compared to calves fed milk replacer [23,24]. However the nutrient value of milk with low total solids (<13%) can be improved by adding milk replacer following assessment of milk total solids. Mean total solids from the samples reported in this study were lower than recommended of levels of 12.5-13% [11,12]. The sensitivity of the refractometer in detecting milk samples with < 12% total solids was perfect. The mean bias of the refractometer (0.6%) indicated that the refractometer underestimated the milk total solids by 0.6%, on average. Based on these results, the refractometer is a recommended method for assessing milk total solids because the underestimation is of smaller magnitude, on average.

Although the colostrum IgG concentrations in this study were variable, it is important to note that only samples from Jersey cows were evaluated. While other studies indicated that colostrum IgG concentrations were not different among five dairy breeds (Holsteins, Jersey, Guernsey, Brown Swiss and Ayrshire) [25], other studies reported significantly higher colostrum IgG concentrations in Guernsey compared to Holsteins under the same management conditions [26]. However considerable within breed variations in colostrum IgG concentrations has been reported in Holsteins [3,27,28] and Jersey cows [29,30]. Thus, it is mostly likely that the variability in colostrum samples in this study from 3 different farms

were sufficient to evaluate the refractometer. It should be noted that the refractometer was assessed in one geographical area, thus the external validity of its performance may vary. Thus it is recommended to individually validate the refractometer in different geographical conditions where colostral IgG, serum IgG or milk solids concentration are different.

## Conclusions

Results of the present study indicated that the use of the single refractometer is an acceptable on-farm method for quantitatively evaluating colostral IgG concentrations and milk total solids in dairy cattle. The refractometer was not an acceptable method for determination of serum IgG concentrations in calves. The refractometer can be used by producers to assess colostral IgG and milk total solids concentrations prior to feeding calves.

## Competing interests

The authors declare that they have no competing interests.

## Authors' contributions

MC conceived the experiment, designed the experiment, performed statistical analysis and wrote the manuscript. JV performed sample analysis and proof read the manuscript. Both authors read and approved the final manuscript.

## Acknowledgements

The authors would like to thank Dr. Elizabeth Adams, Dr. Craig Meadows and Peter Koch for their assistance in collection of samples. The study was funded by the University of California, Davis faculty support funds.

Received: 12 May 2014 Accepted: 4 August 2014

Published: 15 August 2014

## References

1. Fleenor WA, Stott GH: **Hydrometer test for estimation of immunoglobulin concentration in bovine colostrum.** *J Dairy Sci* 1980, **63**:973–977.
2. Pritchett LC, Gay CC, Hancock DD, Besser TE: **Evaluation of the hydrometer for testing immunoglobulin G1 in Holstein colostrum.** *J Dairy Sci* 1994, **77**:1761–1767.
3. Pritchett LC, Gay CC, Besser TE, Hancock DD: **Management and production factors influencing immunoglobulin G<sub>1</sub> concentration in colostrum from Holstein cows.** *J Dairy Sci* 1991, **74**:2336–2341.
4. Chigerwe M, Dawes ME, Tyler JW, Middleton JR, Moore MP, Nagy DM: **Evaluation of a cow-side immunoassay kit for assessing IgG concentration in colostrum.** *J Am Vet Med Assoc* 2005, **227**:129–131.
5. Chigerwe M, Tyler JW, Schultz LG, Middleton JR, Spain JN, Dill JS, Steevens BJ: **Comparison of four methods to assess colostral IgG concentration in dairy cows.** *J Am Vet Med Assoc* 2008, **233**:761–766.
6. Tyler JW, Hancock DD, Wiksie SE, Holler SL, Gay JM, Gay CC: **Use of serum protein concentration to predict mortality in mixed-source dairy replacement heifers.** *J Vet Intern Med* 1998, **12**:79–83.
7. Vandeputte S, Detilleux J, Rollin F: **Comparison of four refractometers for investigation of passive transfer in beef calves.** *J Vet Intern Med* 2011, **25**:1465–1469.
8. Tyler JW, Hancock DD, Parish SM, Rea DE, Besser TE, Sanders SG, Wilson LK: **Evaluation of 3 assays for failure of passive transfer in calves.** *J Vet Intern Med* 1996, **10**:304–307.
9. Alley ML, Haines DM, Smith GW: **Evaluation of serum immunoglobulin G concentrations using an automated turbidimetric immunoassay in dairy calves.** *J Dairy Sci* 2012, **95**:4596–4599.
10. Fahey JL, McKelvey EM: **Quantitative determination of serum immunoglobulin in anti-body agar plates.** *J Immunol* 1965, **94**:84.
11. Foley JA, Otterby DE: **Availability, storage, treatment, composition, and feeding value of surplus colostrum: a review.** *J Dairy Sci* 1978, **61**:1033–1060.
12. Moore DA, Taylor J, Hartman ML, Sischo WM: **Quality assessment of waste milk at a calf ranch.** *J Dairy Sci* 2009, **92**:3503–3509.
13. Hans H, Ersbøll AK, Toft N: **Sample size and sampling methods.** In *Introduction to Veterinary Epidemiology*. Frederiksberg: Biofilia; 2004:109–130.
14. Zar JH: **Power and sample size in correlation.** In *Biostatistical Analysis*. Saddle River: Upper Prentice Hall Inc; 1999:377–410.
15. Wehr HM, Frank JH: **Standard methods for the examination of dairy products.** Washington DC: American Public Health Association; 2004:460–479.
16. Besser TE, Gay CC, Pritchett L: **Comparison of three methods of feeding colostrum to dairy calves.** *J Am Vet Med Assoc* 1991, **198**:419–422.
17. Furman-Fratczak K, Rzasa A, Stefaniak T: **The influence of colostral immunoglobulin concentration in heifer calves' serum on their health and growth.** *J Dairy Sci* 2011, **94**:1536–1539.
18. Altman DG, Bland JM: **Measurement in medicine: the analysis of method comparison studies.** *Statistician* 1983, **32**:307–317.
19. Mohammadi M: **Colloidal refractometry: meaning and measurement of refractive index for dispersions; the science that time forgot.** *Adv Colloid Interface Sci* 1995, **62**:17–29.
20. Fox PF, McSweeney PLH: **Physical properties of milk.** In *Dairy Chemistry and Biochemistry*. New York: Black Academic and Professional; 1998:437–461.
21. Chigerwe M, Tyler JW, Schultz LG, Middleton JR, Steevens BJ, Spain JN: **Effect of colostral administration by use of oesophageal intubation on serum IgG concentrations in Holstein bull calves.** *Am J Vet Res* 2008, **69**:1158–1163.
22. Weaver DM, Tyler JW, VanMetre DC, Hostetler DE, Barrington GM: **Passive transfer of colostral immunoglobulins in calves.** *J Vet Intern Med* 2000, **14**:569–577.
23. Jamaluddin AA, Carpenter TE, Hird DW, Thurmond MC: **Economics of feeding pasteurized colostrum and pasteurized waste milk to dairy calves.** *J Am Vet Med Assoc* 1996, **209**:751–756.
24. Godden SM, Fetrow JP, Feirtag JM, Green LR, Wells SJ: **Economic analysis of feeding pasteurized nonsaleable milk versus conventional milk replacer to dairy calves.** *J Am Vet Med Assoc* 2005, **226**:1547–1554.
25. Muller LD, Ellinger DK: **Colostral immunoglobulin concentrations among breeds of dairy cattle.** *J Dairy Sci* 1981, **64**:1727–1730.
26. Tyler JW, Steevens BJ, Hostetler DE, Holle JM, Denbigh JL: **Colostral immunoglobulin concentrations in Holstein and Guernsey cows.** *Am J Vet Res* 1999, **60**:1136–1139.
27. Burton LJB, Kennedy BW, Burnside BN, Wilke BN, Burton JH: **Variation in serum concentrations of immunoglobulins G, A, and M in Canadian Holstein-Friesian calves.** *J Dairy Sci* 1989, **72**:135–149.
28. Maunsell FP, Morin DE, Constable PD, Hurley WL, McCoy GC: **Use of mammary gland and colostral characteristics for prediction of colostral IgG<sub>1</sub> concentrations and intramammary infection in Holstein cows.** *J Am Vet Med Assoc* 1999, **214**:1817–1823.
29. Logan EF, Meneely DJ, Lindsay A: **Colostrum and serum immunoglobulin levels in Jersey cattle.** *Vet J* 1991, **137**:279–282.
30. Quigley JD, Martin KR, Dowlen HH, Wallis LB, Lamar K: **Immunoglobulin concentration, specific gravity, and nitrogen fractions of colostrum from Jersey cattle.** *J Dairy Sci* 1994, **77**:264–269.

doi:10.1186/s12917-014-0178-7

**Cite this article as:** Chigerwe and Hagey: Refractometer assessment of colostral and serum IgG and milk total solids concentrations in dairy cattle. *BMC Veterinary Research* 2014 **10**:178.