

Lawrence Berkeley National Laboratory

LBL Publications

Title

Research Progress Meeting

Permalink

<https://escholarship.org/uc/item/7k89s1vq>

Author

Wakerling, R K

Publication Date

1948-05-01

Copyright Information

This work is made available under the terms of a Creative Commons Attribution License, available at <https://creativecommons.org/licenses/by/4.0/>

UCRL 114

977/A
C2

RECEIVED

UNIVERSITY OF
CALIFORNIA

*Radiation
Laboratory*

TWO-WEEK LOAN COPY

*This is a Library Circulating Copy
which may be borrowed for two weeks.
For a personal retention copy, call
Tech. Info. Division, Ext. 5545*

BERKELEY, CALIFORNIA

UCRL 114
C2

DISCLAIMER

This document was prepared as an account of work sponsored by the United States Government. While this document is believed to contain correct information, neither the United States Government nor any agency thereof, nor the Regents of the University of California, nor any of their employees, makes any warranty, express or implied, or assumes any legal responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by its trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof, or the Regents of the University of California. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof or the Regents of the University of California.

DECLASSIFIED

~~RESTRICTED~~
UCRL 114

Physics-General

CLASSIFICATION CANCELLED
BY AUTHORITY OF THE DECLASSIFICATION
BRANCH USAEC *REF ID - 1109*
BY *B. J. J. J.* *1-31-76*
SIGNATURE OF THE PERSON MAKING THE CHANGE DATE

UNIVERSITY OF CALIFORNIA

Radiation Laboratory

Contract No. W-7405-eng-48

RESEARCH PROGRESS MEETING

May 27, 1948

R. K. Wakerling

Special Section of Declassified Reports
Authorized by USDOE JX Division
Unclassified TWX P182206Z May 79

REPORT PROPERLY DECLASSIFIED

JN Green *8/16/77*
Authorized Derivative Classifier Date
R K J. J. *8/17/77*
By Date

Berkeley, California

STANDARD DISTRIBUTION: Series A/UCRL 114

Copy Numbers

Argonne National Laboratory	1-8
Armed Forces Special Weapons Project	9
Atomic Energy Commission, Washington	10-11
Battelle Memorial Institute	12
Brookhaven National Laboratories	13-20
Carbide & Carbon Chemicals Corporation (K-25 Area)	21-24
Carbide & Carbon Chemicals Corporation (Y-12 Area)	25-28
Columbia University (Dunning)	29
General Electric Company	30-33
Hanford Directed Operations	34-38
Iowa State College	39
Los Alamos	40-42
Monsanto Chemical Company, Dayton	43-44
National Bureau of Standards	45-46
Naval Radiological Defense Laboratory	47
NEPA	48
New York Directed Operations	49-50
Oak Ridge National Laboratory	51-58
Patent Advisor, Washington	59
Technical Information Division, ORDO	60-74
UCLA Medical Research Laboratory (Warren)	75
University of California Radiation Laboratory	
Information Division	76-78
Chemistry Dept., Bldg 4	79
Patent Dept., Bldg 29	80
University of Rochester	81-82
Chicago Office of Directed Operations	83

TOTAL 83 Copies.

Information Division
Radiation Laboratory
UNIVERSITY OF CALIFORNIA
Berkeley, California

RESEARCH PROGRESS MEETING

May 27, 1948

R. K. Wakerling

Neutron Scattering. A. Bratenahl.

The experiments on the scattering of 90 Mev neutrons have continued with the use of proportional counters in coincidence as detectors. It will be recalled that in the early work stacks of carbon plates were used as detectors. The results for the two methods of measurement agree quite well. However, there exists a difference between the differential scattering cross sections as measured with either system and those predicted by diffraction theory treating the nuclei as opaque obstacles of radii measured by McMillan et al. Intensities in the scattered angles investigated ($0^\circ - 10^\circ$) are higher than the simple diffraction theory would predict. If the tail of the scattering curve is assumed to give the measure of the inelastic scattering and this is subtracted from the observed values, a much better agreement with theory is found.

In Figure 1 is shown schematically the set-up of the apparatus used. Proportional counters are used in triple coincidence with a 60 Mev absorber placed between the second and third counters. A lead house surrounds the counter system at one end and behind it is placed a transition thickness of paraffin for the generation of protons.

One of the major difficulties in the use of proportional counters is the large range of counting rates required. When the counters are first placed in the beam to measure its intensity and then placed in the field of scattered neutrons, the intensity range varies by a factor of a thousand. Since this type of counter system is limited to about 6400 counts per minute, some other system of monitoring

the beam is necessary. The scheme presently employed involves the use of a BF_3 counter placed in the concrete shielding wall adjacent to the collimating hole through which the neutrons emerge. As a check another monitor counter is placed in the concrete igloo at some distance from the shielding wall. Because of the large range of counting rates that can be covered, low backgrounds and good plateaus, this system has been used with fairly satisfactory results. Adjustment of the beam strength is made to provide approximately the same counting rates in the coincidence proportional counters under all conditions, and the monitor counter takes care of the large range of counting rates required.

As mentioned above, the results obtained with this system confirm previous measurements with carbon detectors. In order to test the performance of this system good geometry attenuation data have been taken with copper over an intensity reduction of about 10,000. The half-value thickness found was between 1.6 and 1.7 inches, in agreement with values obtained by Knable using bismuth fission counter detectors. However, it does not agree with the value of 1.45 inches obtained with carbon detectors by McMillan et al. Measurements will be made of the total cross sections of a number of elements in the collimated beam with the coincidence proportional counter apparatus and with an energy threshold at 60 Mev.

Some further total cross section measurements were made outside the shielding with carbon detectors. The following table shows a comparison of these measurements with similar measurements of McMillan, and with others made using the proportional counter technique.

	σt (Carbon detectors)	σt (McMillan et al)	σt (Proportional counter)
Pb	4.74 b	4.53 b	4.53 b
Cu	2.32	2.22	2.12
C	0.535	0.550	0.54

Nuclear Cross Sections. Norman Knable.

Attention is again being given to the problem of measuring total cross sections by the use of bismuth fission counters. A considerable effort has been expended in attempts to improve the instrumentation. Particular care has been exercised in aligning the apparatus with the neutron beam. This was done by taking shadow radiographs of the beam with the apparatus in place. It is felt that this method is more accurate and reliable than that of using the optical system employed for aligning the cloud chamber. To illustrate (see Figure 2), the alignment is such that a brass cylinder placed in the beam as shown in the figure casts a well defined shadow on the photographic plate placed in front of the detector chamber, showing that the neutron paths are aligned parallel to the axis of the cylinder. Similar radiographs were taken with the apparatus in place and with the photographic plate placed at the end of the detector. This method is very quick and establishes with certainty the alignment of the system.

The detector consists of an ionization chamber 18 inches long containing 30 discs 2 inches in diameter. Alternate discs are coated with a 1 milligram per square centimeter deposit of bismuth. A 500 volt potential is established between alternate plates so that particles released from the bismuth are attracted to and deposited on the non-coated plates. Without the absorber in place 1280 counts per minute were obtained. By the use of thin bismuth coatings a plateau in the curve of the counting rate versus pulse height selector is obtained. Figure 3 shows a typical curve. The discriminator voltage is customarily used at 50 volts where the change of counting rate is only 1-1/2 percent per volt. Measurements conducted over a long period of time indicate that the discriminator voltage and the linear amplification are extremely constant so that the apparatus may be run without adjustment for considerable periods of time.

-6-

The scatterer, usually one mean free path in thickness, is placed at a distance of 8 feet from the detector so that the solid angle of scattering detected is only .0004 steradians. Initial measurements on attenuation in copper agree with those obtained by Bratenahl mentioned above, as well as with the early work done last year on this problem. The half-value thickness found was between 1.6 and 1.7 inches. Cross sections measured thus far are given in the following table as compared with earlier measurements of McMillan et al.

	McMillan	Attenuation measurement	Scattering through 1 MFP of material
H	.083 b	.079 b	
Be	.431		.396 b
C	.550	.450	.502
O	.765	.660	
Al	1.12	.957	
Cu	2.22	1.89	2.00
Sn	3.28	3.02	3.13
Pb	4.53		4.38
U	5.03	5.06	

LMB/6-2-48
Information Div.

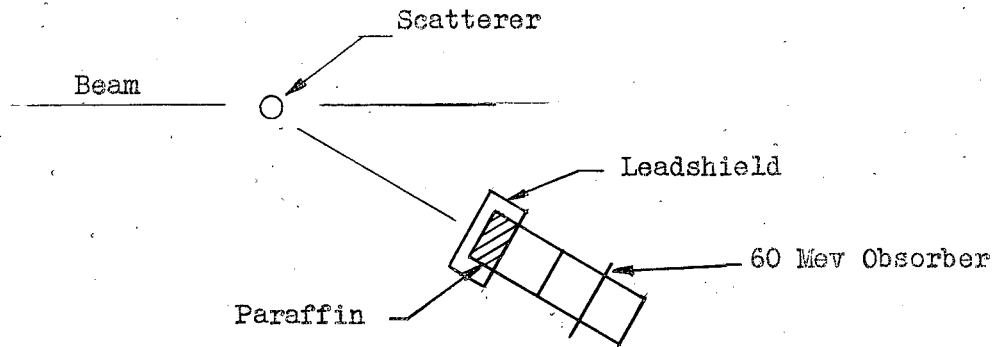


Figure 1

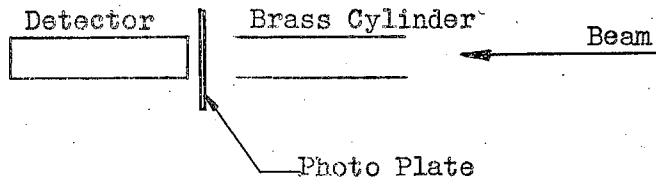


Figure 2

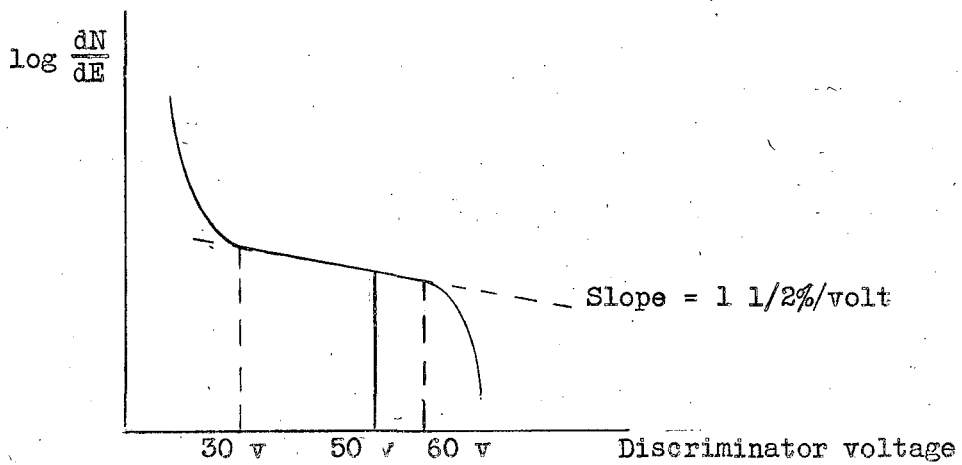


Figure 3

RESTRICTED