



# Lawrence Berkeley Laboratory

UNIVERSITY OF CALIFORNIA

## APPLIED SCIENCE DIVISION

Submitted to Health Physics


Non-Emanating Samples of the Rn Series from  $^{226}\text{Ra}$ ,  
 $^{228}\text{Th}$ , and  $^{227}\text{Ac}$

L.S. Ruzer

December 1989

**For Reference**

Not to be taken from this room

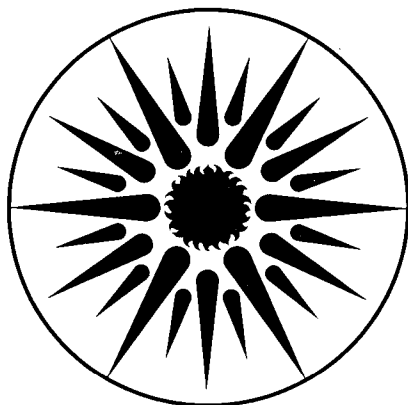

**APPLIED SCIENCE  
DIVISION**

## **DISCLAIMER**

This document was prepared as an account of work sponsored by the United States Government. While this document is believed to contain correct information, neither the United States Government nor any agency thereof, nor the Regents of the University of California, nor any of their employees, makes any warranty, express or implied, or assumes any legal responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by its trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof, or the Regents of the University of California. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof or the Regents of the University of California.

Submitted to  
*Health Physics*

**NON-EMANATING SAMPLES OF THE Rn SERIES  
FROM  $^{226}\text{Ra}$ ,  $^{228}\text{Th}$  AND  $^{227}\text{Ac}$**

L.S. Ruzer  
Indoor Environment Program  
Applied Science Division  
Lawrence Berkeley Laboratory  
Berkeley, CA 94720 USA

December 1989

This work was supported by the Director, Office of Energy Research, Office of Health and Environmental Research, Human Health Assessments Division and Pollutant Characterization and Safety Research Division of the U.S. Department of Energy under Contract No. DE-AC03-76SF00098.

# NON-EMANATING SAMPLES OF THE Rn SERIES FROM $^{226}\text{Ra}$ , $^{228}\text{Th}$ AND $^{227}\text{Ac}$

L.S. Ruzer

Aerosol Department, All-Union Institute of  
Physico-Technical and Radiotechnical Measurements, Moscow, U.S.S.R.\*

Key words:  $^{222}\text{Rn}$ , decay-product samples, calibration, alpha sources

The short-lived decay products of  $^{222}\text{Rn}$  are  $^{218}\text{Po}$  and  $^{214}\text{Po}$ ,  $\alpha$ -emitters with energies of 6.00 and 7.69 MeV, respectively, and  $^{214}\text{Pb}$  and  $^{214}\text{Bi}$ ,  $\beta$ -emitters that include branches with endpoint energies of 0.64 and 3.27 MeV, respectively. Because of the considerable difference between the energies of each pair of these radionuclides, the concentration of decay products in the air can be measured with good accuracy by means of portable scintillating or semiconductor spectrometers (Ruzer and Labushkin 1965, Labushkin and Ruzer 1965, Nazaroff 1988).

In order to determine decay-product concentrations accurately, it is necessary to calibrate the appropriate equipment by one of three methods: by producing standard aerosols of radon decay products, by fabricating standard samples of the decay products, or by using other types of sources that yield radiation of the appropriate type and energy range.

The last approach is the most common, but suffers the disadvantage of utilizing radiation that does not correspond exactly to that emitted by the decay products. On the other hand, use of a decay-product aerosol in an environmental chamber -- while the ultimate controlled test of the performance of a decay product monitoring technique -- is inconvenient for normal calibration purposes. The ideal technique for most purposes would be a long-lasting decay-product source having a configuration that is similar to that in which decay products are typically collected in the actual monitoring device, i.e., on a filter. However, due to the small half-life of the radon decay products, fabrication of such a sample presents great difficulties.

Nonetheless, a cooperative effort between our Institute and the Radium Institute in Leningrad has succeeded in producing non-emanating samples of each of the Rn decay series (Volkova et al. 1966). Each sample consists of a foil onto which is deposited, first, a substance that retains Rn with 95 - 97% efficiency, then a thin layer of the appropriate long-lived parent radionuclide (in a solution that is evaporated), and finally a thin foil to retain the 3 - 5% of Rn that would otherwise emanate. The peak width (FWHM) due to loss in the source is  $\leq 50$  keV. Samples with activities in the range 40 to 4000 Bq have been fabricated with areas from 5 to 20 cm<sup>2</sup>.

---

\* Present address: Indoor Environment Program, Applied Science Division, Lawrence Berkeley Laboratory, Berkeley, CA 94720.

Figure 1 shows  $\alpha$  spectra from a  $^{222}\text{Rn}$ -series sample fabricated in this manner from a  $^{226}\text{Ra}$  solution. The spectra were obtained using a scintillation spectrometer (a  $\text{CsI(Tl)}$  crystal with a thickness of  $\sim 100\mu\text{m}$ ) with resolution 3.5% and a semiconductor (Si) detector with resolution 0.5%, i.e., approximately 30 keV. Samples of this type and quality can greatly simplify calibration of decay-product measurement devices. A similar non-emanating sample has been developed for the  $^{220}\text{Rn}$  and  $^{219}\text{Rn}$  series together, yielding spectra such as seen in Figure 2. Such non-emanating samples have been used for many years with no sign of deterioration or leakage of Rn.


Non-emanating samples of this kind can be useful in measuring concentrations of decay products of each of the  $^{222}\text{Rn}$ ,  $^{220}\text{Rn}$  and  $^{219}\text{Rn}$  series, as well as in studies of the unattached fraction of  $^{218}\text{Po}$ . They can also be used for more general purposes, such as for calibrating instruments for measuring concentrations of artificial radioactive aerosols such as  $^{239}\text{Pu}$  and  $^{210}\text{Po}$  and for linearity testing and energy-resolution measurement for a wide range of  $\alpha$  energies.

The author wants to express his gratitude to Dr. Anthony Nero for discussion and help in preparation of this article and to the U.S. Department of Energy's Office of Health and Environmental Research for assistance in its preparation.

## REFERENCES


- Browne, E.; Firestone, R.B. *Table of Radioactive Isotopes* (V.S. Shirley, ed). New York: Wiley-Interscience; 1986.
- Labushkin, V.G.; Ruzer, L.S. A method of determining the concentrations of short-lived daughters products of radon in air by the  $\alpha$ - and  $\beta$ - radiations. *Atonmaja Energia*, 19:24-28; 1965.
- Nazaroff, W.W. Measurement techniques. In: *Radon and its Decay Products in Indoor Air* (Nazaroff, W.W. and Nero, A.V., eds.). New York: Wiley-Interscience; 1988: 491-504.
- Ruzer, L.S.; Labushkin, V.G. Author's Certificate No. 171478, Method of determination of concentration of short-lived radon daughters decay products. *Buyl. of Inventions*, U.S.S.R. (in Russian) N11; 1966.

Volkova, E.A., Ziv, D.U., Labushkin, V.G., Ruzer, L.S., Stepanov, E.K., Tyutikov, N.V.  
Determination of the Parameter of  $\alpha$ -spectrometers with  $^{226}\text{Ra}$  and  $^{228}\text{Th}$  sources. *Pribory  
i Teknika Eksperimenta*, 4:36-39; 1966.

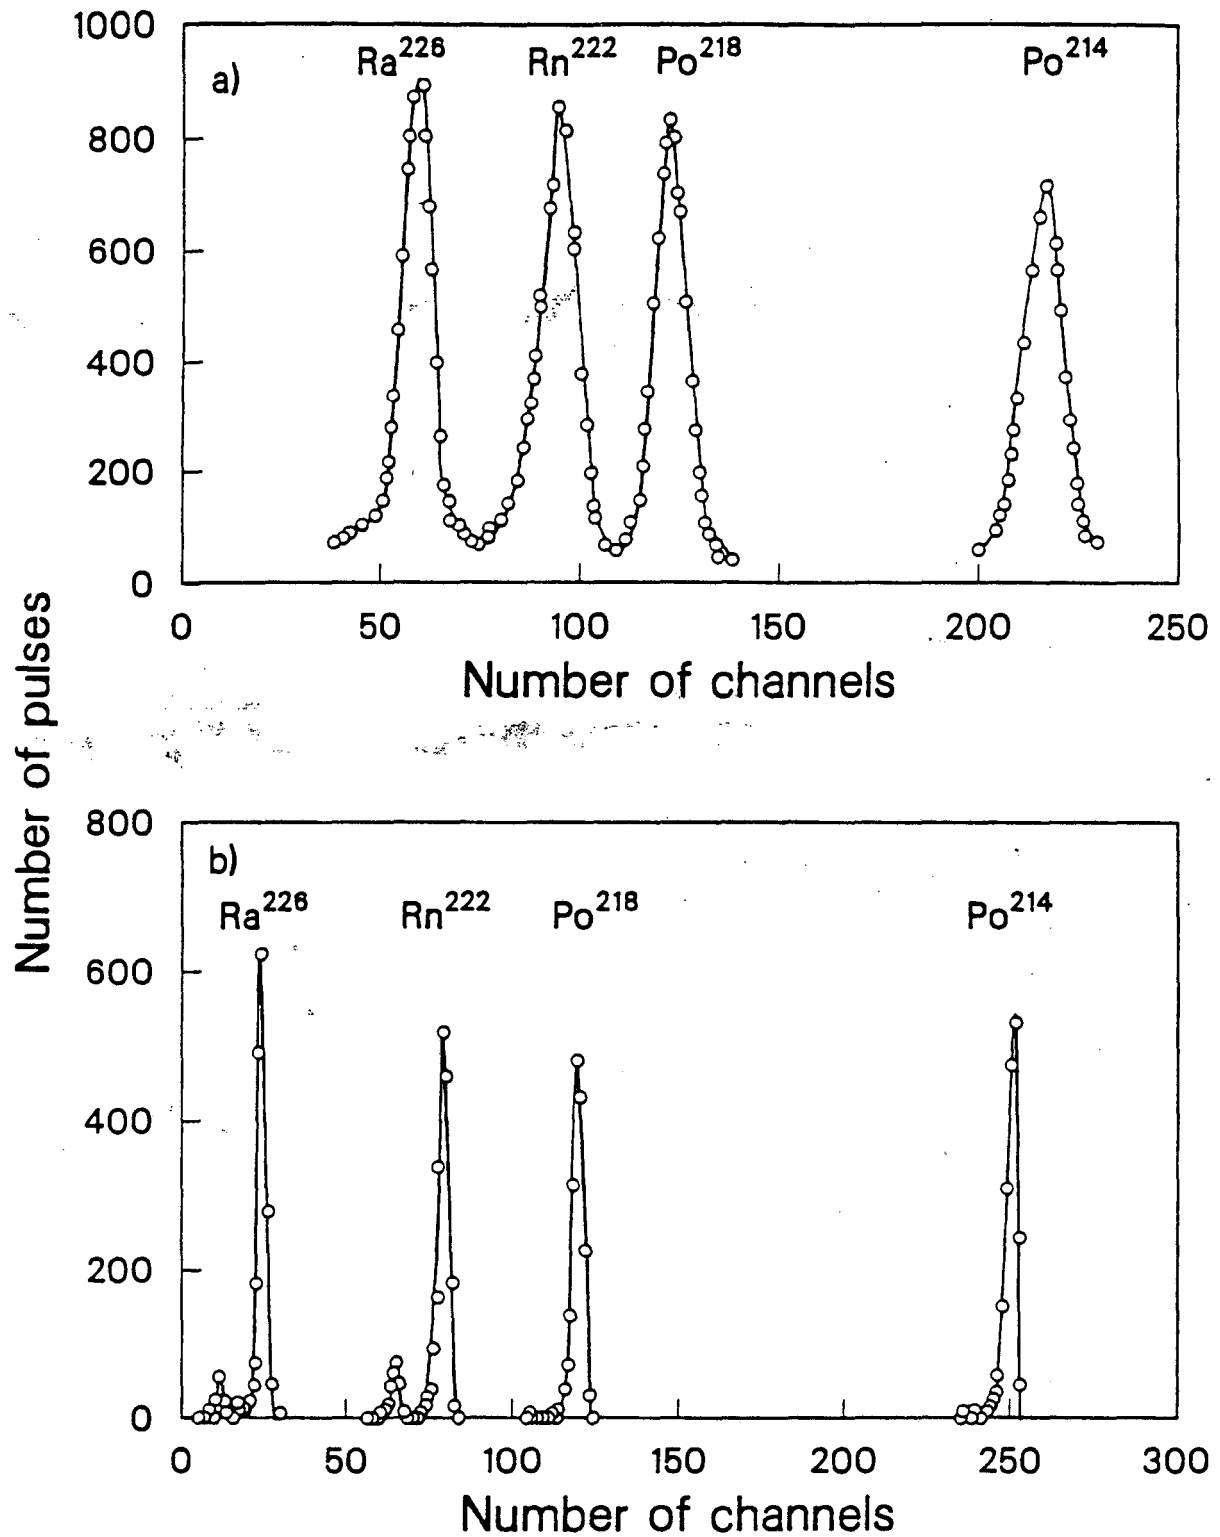

XCG 893-4640

Figure 1: Alpha spectra from a  $^{222}\text{Rn}$ -series non-emanating sample. The upper spectrum was obtained using a CsI(Tl) scintillator, the lower a semiconductor detector. The small unidentified peak to the left of the  $^{222}\text{Rn}$  peak (lower spectrum) is due to the 5.3-MeV  $\alpha$  particle from  $^{210}\text{Po}$ , which has grown into the sample over a period of more than a year.

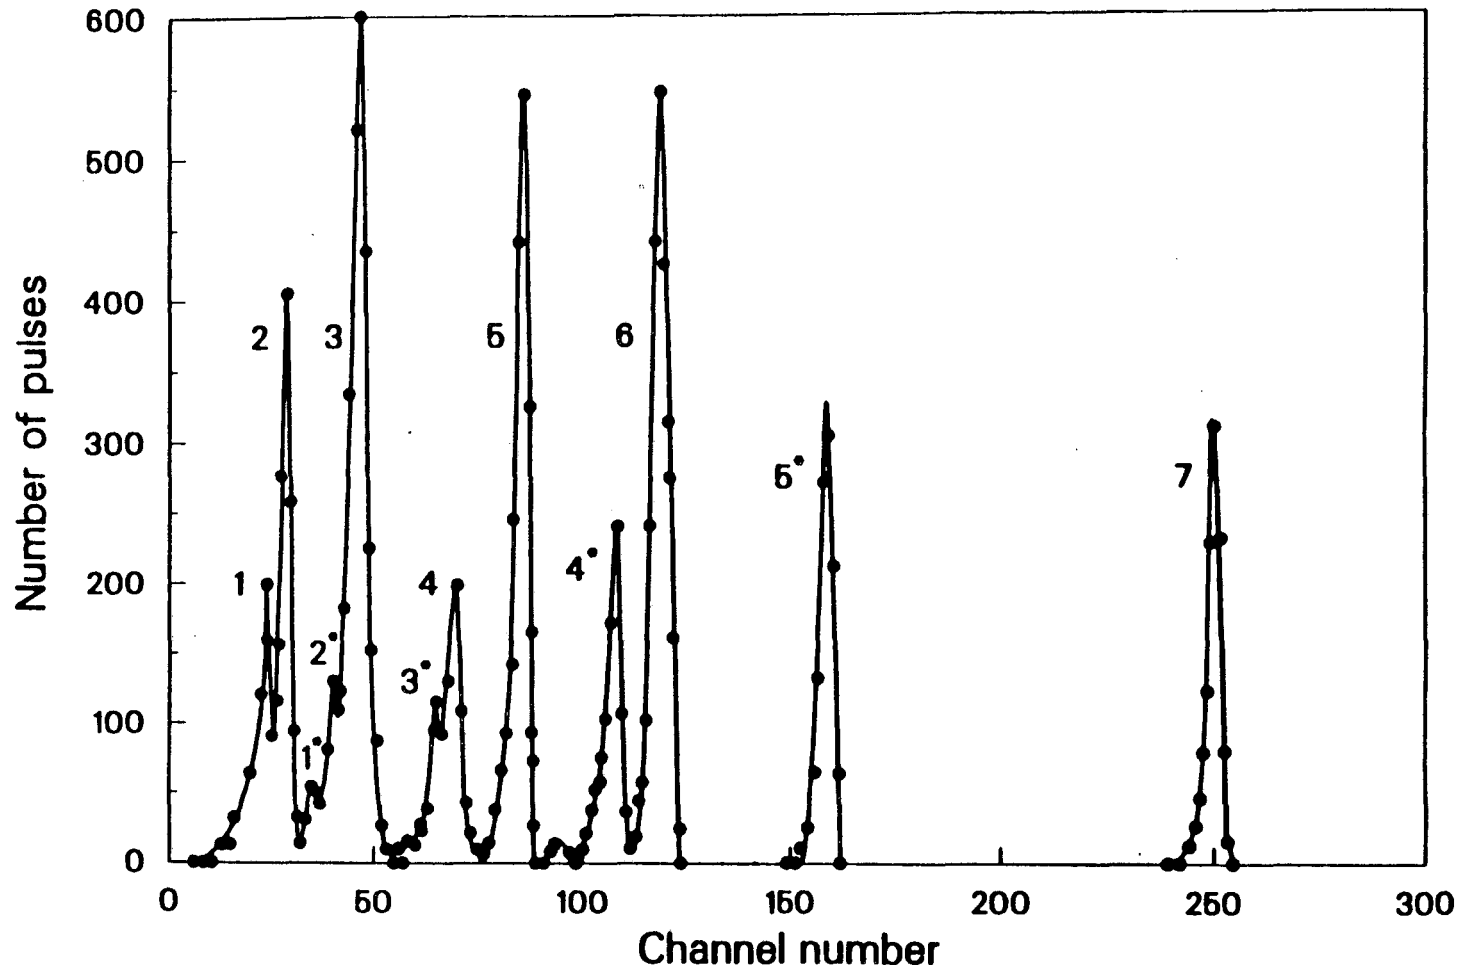

XCG 893-4643

Figure 2: Alpha spectrum from a  $^{220}\text{Rn}$  and  $^{219}\text{Rn}$  series sample obtained using a semiconductor detector. The numbered peaks correspond to the following  $\alpha$  particles: in the  $^{228}\text{Th}$  ( $^{220}\text{Rn}$ ) series -- peaks 1 and 2, 5.34 and 5.42 MeV (from  $^{228}\text{Th}$ ); peak 3, 5.45 and 5.69 MeV ( $^{224}\text{Ra}$ ); peak 4, 6.05 MeV ( $^{212}\text{Bi}$ ); peak 5, 6.29 MeV ( $^{220}\text{Rn}$ ); peak 6, 6.78 MeV ( $^{216}\text{Po}$ ); and peak 7, 8.78 MeV ( $^{212}\text{Po}$ ) -- and in the  $^{227}\text{Ac}$  ( $^{219}\text{Rn}$ ) series -- peaks 1\* and 2\*, 5.61 and 5.71 MeV ( $^{223}\text{Ra}$ ); peak 3\*, 5.90 MeV ( $^{227}\text{Th}$ ); peak 4\*, 6.55 MeV ( $^{211}\text{Bi}$ ); and peak 5\*, 7.39 MeV ( $^{215}\text{Po}$ ). (Alpha energies here and in text taken from Browne and Firestone 1986.)



LAWRENCE BERKELEY LABORATORY  
TECHNICAL INFORMATION DEPARTMENT  
1 CYCLOTRON ROAD  
BERKELEY, CALIFORNIA 94720